

BEST AVAILABLE COPY

REC'D 19 MAR 2003

P1 973581

THE UNITED STATES OF AMERICA

TO ALL TO WHOM THESE PRESENTS SHALL COME:

UNITED STATES DEPARTMENT OF COMMERCE
United States Patent and Trademark Office

March 12, 2003

THIS IS TO CERTIFY THAT ANNEXED HERETO IS A TRUE COPY FROM
THE RECORDS OF THE UNITED STATES PATENT AND TRADEMARK
OFFICE OF THOSE PAPERS OF THE BELOW IDENTIFIED PATENT
APPLICATION THAT MET THE REQUIREMENTS TO BE GRANTED A
FILING DATE.


APPLICATION NUMBER: 10/098,601

FILING DATE: March 15, 2002

RELATED PCT APPLICATION NUMBER: PCT/US03/02142



By Authority of the
COMMISSIONER OF PATENTS AND TRADEMARKS


H. PHILLIPS
Certifying Officer

PRIORITY DOCUMENT
SUBMITTED OR TRANSMITTED IN
COMPLIANCE WITH
RULE 17.1(a) OR (b)

03-18-2

A

PTO/SB/13/PCT (10-00)

Approved for use through 10/31/2002. OMB 0651-0032
U.S. Patent and Trademark Office; U.S. DEPARTMENT OF COMMERCE

Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it displays a valid OMB control number.

Request For Filing A Continuation Or Division Of An International Application

DOCKET NUMBER	ANTICIPATED CLASSIFICATION OF THIS APPLICATION		PRIOR APPLICATION EXAMINER	ART UNIT
32355.12.1.2	CLASS	SUBCLASS		

Address to:

Commissioner for Patents
Washington, D.C. 20231

This is a request for filing a ☒ continuation ☐ divisional application under 37 CFR 1.53(b) of pending prior international application Number PCT/US01/41908, filed on 28 August 2001, entitled METHOD AND SYSTEM FOR MAMMALIAN JOINT RESURFACING (which designated the United States), and which in turn claims priority from provisional patent application having United States Serial No. 60/228,444, filed 28 August 2000.

Note: 37 CFR 1.53(d) cannot be used to file a continuation or divisional application of an international application which has not entered the national stage.

CLAIMS	(1) FOR	(2) NUMBER FILED	(3) NUMBER EXTRA	(4) RATE	(5) CALCULATIONS
	TOTAL CLAIMS (37 CFR 1.16(c))	83 - 20 =	63	X \$ 18.00=	\$1134.00
	INDEPENDENT CLAIMS (37 CFR 1.16(b))	3 - 3 =	0	X \$ 84.00=	\$ 0
	MULTIPLE DEPENDENT CLAIMS (if applicable) (37 CFR 1.16(d))			+ \$280.00=	\$ 280.00
	BASIC FEE (37 CFR 1.16(a))				+ \$ 740.00
	Total of above Calculations =				\$2154.00
	Reduction by 50% for filing by small entity (Note 37 CFR 1.27).				\$1077.00
	Total =				\$1077.00

- Enclosed are the specification, claims and eleven (11) sheets of drawings.
- ☒ Applicant claims small entity status. See 37 CFR 1.27.
- ☒ The Commissioner is hereby authorized to charge any fees which may be required under 37 CFR 1.16 and 1.17, or credit any overpayment to Deposit Account No. 061910. A duplicate copy of this sheet is enclosed.
- ☒ A check in the amount of \$1077.00 is enclosed.
- ☐ Payment by credit card. Form PTO-2038 is attached.
- ☒ Application Data Sheet is enclosed. See 37 CFR 1.76.
- ☐ Amend the specification by inserting before the first line the sentence: "This application is a ☐ continuation ☐ division of international application number _____, filed _____ (status, pending)."

[Page 1 of 2]

Burden Hour Statement: This form is estimated to take 0.5 hours to complete. Time will vary depending upon the needs of the individual case. Any comments on the amount of time you are required to complete this form should be sent to the Chief Information Officer, U.S. Patent and Trademark Office, Washington, DC 20231. DO NOT SEND FEES OR COMPLETED FORMS TO THIS ADDRESS. SEND TO: Assistant Commissioner for Patents, Washington, DC 20231.

03/15/02
J1042 PTO1098601
10/098601
J0971 U.S. PTO

10098601.031502

REQUEST FOR FILING A CONTINUATION OR DIVISION OF AN INTERNATIONAL APPLICATION

8. ☐ A declaration under 37 CFR 1.63 is enclosed.
9. ☐ Priority of foreign application number _____, filed on _____ in _____ is claimed under 35 U.S.C. 119(a)-(d).
- ☐ The certified copy is enclosed.
10. ☐ A preliminary amendment is enclosed.
11. ☒ Also enclosed: Return Receipt Postcard


Address all future correspondence to: (May only be completed by applicant, or attorney or agent of record).

Philip M. Goldman, FREDRIKSON & BYRON, P.A., 1100 International Centre,
900 2nd Ave. South, Minneapolis, MN 55402
Customer No. 022859

WARNING: Information on this form may become public. Credit card information should not be included on this form. Provide credit card information and authorization on PTO-2038.

15 MAR 2002

Date

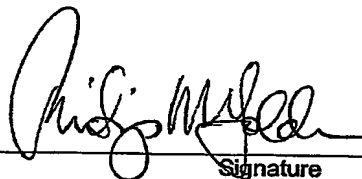

Signature

Philip M. Goldman, Reg. No. 31,162
Typed or printed name

- ☐ Inventor(s)/Applicant(s)
- ☐ Assignee of the entire interest. See 37 CFR 3.71. Statement under 37 CFR 3.73(b) is enclosed. (Form PTO/SB/96).
- ☒ Attorney or agent of record
- ☐ Filed under 37 CFR 1.34(a)
Registration number if acting under 37 CFR 1.34(a). _____

NOTE: Signatures of all the inventors or assignees of record of the entire interest or their representative(s) are required. Submit multiple forms if more than one signature is required, see below*.

☐ *Total of _____ forms are submitted.

**SENT VIA EXPRESS MAIL POST OFFICE TO ADDRESSEE
MAILING LABEL NO. EV049823064US**

::ODMA\PCDOCS\FBDOCS\1\2628994\1

[Page 2 of 2]

Burden Hour Statement: This form is estimated to take 0.5 hours to complete. Time will vary depending upon the needs of the individual case. Any comments on the amount of time you are required to complete this form should be sent to the Chief Information Officer, U.S. Patent and Trademark Office, Washington, DC 20231. DO NOT SEND FEES OR COMPLETED FORMS TO THIS ADDRESS. SEND TO: Assistant Commissioner for Patents, Washington, DC 20231.

APPLICATION DATA SHEET

Inventor Information

Inventor One Given Name: Jeffrey C.
Family Name: FELT
Name Suffix:
Postal Address Line One: 4800 Lodge Lane
Postal Address Line Two:
City: Greenwood
State or Province: Minnesota
Country: United States of America
Postal or Zip Code: 55331
City of Residence: Greenwood
State or Prov. of Residence: Minnesota
Country of Residence: United States of America
Citizenship Country: United States of America

Inventor Two Given Name: Mark A.
Family Name: RYDELL
Name Suffix:
Postal Address Line One: 516 Turnpike Road
Postal Address Line Two:
City: Golden Valley
State or Province: Minnesota
Country: United States of America
Postal or Zip Code: 55416
City of Residence: Golden Valley
State or Prov. of Residence: Minnesota
Country of Residence: United States of America
Citizenship Country: United States of America

Inventor Three Given Name: Paul J.
Family Name: BUSCEMI
Name Suffix:
Postal Address Line One: 2310 Tamarack Drive
Postal Address Line Two:
City: Long Lake
State or Province: Minnesota
Country: United States of America
Postal or Zip Code: 55356
City of Residence: Long Lake
State or Prov. of Residence: Minnesota
Country of Residence: United States of America
Citizenship Country: United States of America

10098601 01500
205100 "T098600T

10098601-031502
205750-1098602

Inventor Four Given Name:

Alexander

Family Name:

ARSENYEV

Name Suffix:

Postal Address Line One:

1845 Turquoise Trail

Postal Address Line Two:

City:

Eagan

State or Province:

Minnesota

Country:

United States of America

Postal or Zip Code:

55122

City of Residence:

Eagan

State or Prov. of Residence:

Minnesota

Country of Residence:

United States of America

Citizenship Country:

Russia

Inventor Five Given Name:

Christopher H.

Family Name:

PORTER

Name Suffix:

Postal Address Line One:

19756 NE 127th Place

Postal Address Line Two:

City:

Woodinville

State or Province:

Washington

Country:

United States of America

Postal or Zip Code:

98072

City of Residence:

Woodinville

State or Prov. of Residence:

Washington

Country of Residence:

United States of America

Citizenship Country:

United States of America

Correspondence Information

Name Line One:

Philip M. Goldman

Address Line One:

Fredrikson & Byron, P.A.

Address Line Two:

900 Second Avenue South

City:

Minneapolis

State or Province:

Minnesota

Postal or Zip Code:

55402

Telephone:

612-347-7088

Fax:

612-347-7077

E-Mail:

pgoldman@fredlaw.com

Application Information

Title Line One:

METHOD AND SYSTEM FOR

Title Line Two:

MAMMALIAN JOINT RESURFACING

Total Drawing Sheets: Eleven (11)
Formal Drawings:
Application Type: utility
Docket Number: 32355.12.1.2
Licensed - U S Government Agency:
Contract Number:
Grant Number:
Secrecy Order in Parent Application:

Representative Information

Representative Customer Number: N/A

Continuity Information

This application is a: Continuation
> Application One: PCT/US01/41908
Filing Date: 28 August 2001
Patent Number:
which is a: claims priority from
>> Application Two :: 60/228,444
Filing Date: 28 August 2000
Patent Number:

Prior Foreign Applications

Foreign Application One: N/A
Filing Date:
Country:
Priority Claimed:

10098601-031502

METHOD AND SYSTEM FOR MAMMALIAN JOINT RESURFACING

5

CROSS REFERENCE TO RELATED APPLICATIONS

The present application is a continuation of an international patent application filed 28 August 2001 and assigned Serial No. PCT/US01/41908 which application has not yet been published and which itself is a continuation-in-part of Provisional US Application Serial No. 60/228,444, filed August 28, 2000, the entire disclosures of which are incorporated herein by reference.

10

TECHNICAL FIELD

In one aspect, this invention relates to biomaterials formed *ex vivo* for implantation and use within the body. In another aspect, the invention relates to *in situ* curable biomaterials. In yet another aspect, this invention further relates to the field of orthopedic implants and prostheses, and more particularly, for implantable materials for use in orthopedic joints.

BACKGROUND OF THE INVENTION

20

Applicant has previously described, *inter alia*, prosthetic implants formed of biomaterials that can be delivered and finally cured *in situ*, e.g., using minimally invasive techniques. See for instance, U.S. Patent Nos. 5,556,429, 5,795,353, 5,888,220, 6,079,868, 6,140,452, 6,224,630 and 6,248,131 as well as published International Application Nos. WO 95/30388 and WO 97/26847 and International Application PCT/US97/20874 filed 11/14/97 (the disclosures of each

of which are incorporated herein by reference). Certain of these applications describe, *inter alia*, the formation of a prosthetic nucleus within an intervertebral disc by a method that includes, for instance, the steps of inserting a collapsed mold apparatus (which in a preferred embodiment is described as a "balloon") through a cannula that is itself positioned through an opening within the annulus, and filling the balloon with a flowable biomaterial that is adapted to finally cure *in situ* and provide a permanent disc replacement. See also, Applicant's "Porous Biomaterial and Biopolymer Resurfacing System" (PCT/US99/10004), as well as "Implantable Tissue Repair Device (PCT/US99/11740), and "Static Mixer" (PCT/US99/04407) applications.

See also, US Patent Nos. 3,030,951 (Mandarino), 4,203,444 (Bonnell et al.), 4,456,745 (Rajan), 4,463,141 (Robinson), 4,476,293 (Robinson), 4,477,604 (Oechsle, III), 4,647,643 (Zdrahala), 4,651,736 (Sanders), 4,722,948 (Sanderson), 4,743,632 (Marinovic et al.), 4,772,287 (Ray et al.), 4,808,691 (König et al.), 4,880,610 (Constanz), 4,873,308 (Coury et al.), 4,969,888 (Scholten et al.), 5,007,940 (Berg), 5,067,964 (Richmond et al.), 5,082,803 (Sumita), 5,108,404 (Scholten et al.), 5,109,077 (Wick), 5,143,942 (Brown), 5,166,115 (Brown), 5,254,662 (Szycher et al.), 5,278,201 (Dunn et al.), 5,525,418 (Hashimoto et al.), 5,624,463 (Stone et al.), 6,206,927 (Fell), and EP 0 353 936 (Cedar Surgical), EP 0 505 634 A1 (Kyocera Corporation), EP 0 521 573 (Industrial Res.), and FR 2 639 823 (Garcia), WO 93/11723 (Regen Corporation), WO 9531946 (Milner), WO 9531948 (Kuslich).

Applicant's PCT Application No. PCT/US97/00457 (WO 9726847A1) includes the optional use of a mold, such as a balloon, and describes the manner in which "[t]he mold created within the joint is preferably of sufficient shape and dimensions to allow the resulting cured biomaterial to replace or mimic the structure and function of the removed fibrocartilage. The mold can be formed of synthetic and/or natural materials, including those that are provided

exogenously and those provided by the remaining natural tissues. The mold can either be removed from the site, upon curing of the biomaterial, or is sufficiently biocompatible to allow it to remain in position."

Applicant's later PCT Application No. PCT/US97/20874 (WO 9820939A2) further describes the manner in which " 'mold' will refer to the portion or portions of an apparatus of the invention used to receive, constrain, shape and/or retain a flowable biomaterial in the course of delivering and curing the biomaterial *in situ*. A mold may include or rely upon natural tissues (such as the annular shell of an intervertebral disc) for at least a portion of its structure, conformation or function. The mold, in turn, is responsible, at least in part, for determining the position and final dimensions of the cured prosthetic implant. As such, its dimensions and other physical characteristics can be predetermined to provide an optimal combination of such properties as the ability to be delivered to a site using minimally invasive means, filled with biomaterial, and optionally, then remain in place as or at the interface between cured biomaterial and natural tissue. In a particularly preferred embodiment the mold material can itself become integral to the body of the cured biomaterial."

Applicant's own use of such mold apparatuses to date has concentrated largely on the use of thin, extensible balloons adapted to be positioned and then filled *in situ* with curable biomaterial, with particular use as a replacement for the intervertebral disc following microdiscectomy. In turn, there has been considerably less focus, to date, on the use of any such molds in other joints, such as the knee. Figures 6 and 7 of Applicant's PCT Publication No. WO 920939 A2, for instance, shows a balloon and corresponding drilling template for use in knee surgery, the balloon having foot portions protruding from a generally ovoid inflatable portion.

Finally, US Patent No. 6,206,927 describes a self-centering meniscal prosthesis device suitable for minimally invasive, surgical implantation into the cavity between a femoral condyle and the corresponding tibial plateau is composed of a hard, high modulus material shaped such that the contour of the device and the natural articulation of the knee exerts a restoring force on the free-floating device. In what appears to be a related manner, Sulzer has introduced a unicompartamental interpositional spacer to treat osteoarthritis in the knee. See "Little Device Could Pack a Big Punch", Sulzer Medica Journal Edition 2/2000 (www.sulzermedica.com/media/smj-full-tex/2000/0002-full-text-6.html). The device is described as a metallic kidney-shaped insert which fills in for the damaged cartilage between the femur and the tibia.

Such a metallic device, as described in either the Fell patent and/or Sulzer's product literature, is described as appropriate for use in younger patients with moderate to severe chondromalacia, particularly since the product provides a hard, self-centering meniscal device that is "devoid of physical means that fix its location". In so doing, the device of Fell et al. tends to require a significant amount of intact cartilage and meniscus. Applicant's own products to date, including those improved embodiments described herein, have been largely geared toward more elderly patients, where such healthy cartilage is lacking. In turn, Applicant's devices tend to provide angular correction and improved anchoring of the implant at the joint surface.

In spite of developments to date, there remains a need for a joint prosthesis system that provides an optimal combination of properties such as ease of preparation and use, and performance within the body.

BRIEF DESCRIPTION OF THE DRAWING

In the Drawing:

Figure 1 shows top and side perspectives of a preferred preformed knee implant prepared according to the present invention.

5 Figure 2 shows an embodiment in which preformed components adapted to be inserted and assembled *in situ*.

Figure 3 shows an alternative embodiment in which preformed components are employed.

Figures 4 and 5 show an embodiment in which a substantially open (saucer-shaped) mold is inserted into the joint site, to be filled with a corresponding curable biomaterial *in situ*.

Figure 6 shows a variety of alternative embodiments that include one or more preformed component.

Figure 7 shows a variety of alternative means for anchoring a preformed component such as that shown in Fig. 6d.

Figure 8 shows a further variety for anchoring or stabilizing a preformed portion by the use of ancillary portions and/or surface texture.

Figure 9 shows a variety of embodiments in a substantially closed (balloon like) mold is adapted to be inserted into the joint site and filled with a corresponding curable biomaterial.

Figure 10 shows a mold adapted for use as an acetabular mold in connection with the
20 replacement of the articulating surface in a hip.

Figure 11 shows a patella femoral joint form suitable for use in combination with the method and system of this invention.

SUMMARY OF THE INVENTION

The present invention provides a method and system for the creation or modification of the wear surface of orthopedic joints, and particularly articulating joints such as the knee. In one preferred embodiment, the method relies, at least in part, upon the manner in which the various stages of curing a curable biomaterial, and in turn, the various stages of forming a component from the cured or curing biomaterial, can be correlated and optimized in a desired manner. In turn, such a method provides the ability to both generally and specifically form the component for use *in situ*.

The present invention includes a variety of embodiments, each of which preferably includes one or more components that are formed *ex vivo*, and that are adapted to be inserted and finally formed or assembled *in situ* in order to provide a final prosthesis and articulating joint surface. Examples of the various embodiments include, for instance,

1) one or more components that are each partially molded *ex vivo*, in a manner that permits the component to be inserted and finally formed *in situ*,

2) a plurality of preformed components adapted to be assembled *in situ*, for instance in an overlapping or interlocking fashion,

3) an insertable open (e.g., saucer shaped) mold, adapted to be inserted and positioned within the joint site, and there used in combination with a flowable biomaterial adapted to be delivered to the open mold *in situ*, under conditions that permit the flowable biomaterial to cure in contact and/or combination with the mold in order to form a final prosthesis,

4) one or more generally extensible envelope (e.g., balloon- type) molds, adapted to be positioned and filled *in situ* with corresponding curable biomaterials, one or more of the molds themselves providing one or more regions of generally non-extensible, preformed material. In

one embodiment, for instance, a plurality of such envelope portions (e.g., a bi-compartmental single envelope) can be adapted for use on both the medial and lateral tibial surfaces, respectively.

By the selection and use of a suitable biomaterial, and other features as described herein, the present invention provides an optimal combination of benefits, as compared to methods previously described. Such benefits include those that arise in the course of preparation and storage (e.g., sterility, storage stability), those that arise in the surgical field itself (e.g., ease of use, adaptability, predictability), and those that arise in the course of long term use within the body (e.g., biocompatibility, moisture cure characteristics, tissue congruity and conformability, retention, wear characteristics, and physical-mechanical properties).

In one preferred embodiment, the method and system involve the preparation and use of partially cured components that can be formed outside the body, for insertion and placement into the body, and that can then be further formed within the joint site in order to enhance conformance. The ability to finally form one or more components *in situ* provides various additional benefits, such as increased control over the overall size and shape of the final prosthesis, improved shape and compliance of the surface apposing natural bone, and finally, improved shape and compliance of the opposite, articulating surface.

As used herein, the word "cure", and inflections thereof, will refer to the extent to which a curable biomaterial, as used to form a component of this invention, has begun or completed whatever physical- chemical reactions may be contemplated in the course of fully forming the component, at the surgical site, for long term use *in situ*. In turn, the biomaterial can be considered as uncured (as in component parts that have not yet been mixed or compositions that have not yet been activated), or it can be partially cured (e.g., wherein the components have been

mixed, or compositions activated, under conditions suitable to begin the curing process), or it can be fully cured (e.g., in which case, whatever chemical reactions may have occurred have substantially subsided). Generally, uncured compositions are sterile, storage stable, and often flowable, though are typically not yet formed or capable of being formed.

5 Curing compositions, by contrast, generally begin as flowable compositions, but become nonflowable over a finite time period as they begin to gel or set. Curing compositions can also be minimally formed, e.g., outside the body by the use of molds and/or suitable shaping tools, and/or within the body, as by the initial positioning of the component on supporting bone and by the repositioning of opposing, articulating bone surfaces. Thereafter, it is contemplated that certain compositions of this invention can be further formed, over time, as by the gradual effect of articulating bone in the course of long term use.

As also used herein, the word "form", and inflections and variations thereof, will refer to the manner and extent to which a component has been sized and shaped, in either a general and/or specific manner, for use at a joint site. In turn, the forming of such a component can occur either *ex vivo* and/or *in vivo*, as well as in a general manner (e.g., by the use of an *ex vivo* mold or tools) and/or a specific manner (e.g., by final curing in apposition to supporting bone and/or opposing articulating bone surfaces), as well as combinations thereof.

A component can be "specifically" formed in this manner in order to conform the component (and particularly its surfaces) to the corresponding specific shapes and dimensions of
20 bone *in situ*, including both supporting bone surfaces and/or opposing (e.g., articulating) bone surfaces. Such specific conformation, in turn, can be used to improve a variety of characteristics of the final implant, including comfort, mechanical performance, and/or long term stability. Such conformation can also include aspects in which one or more components, or the composite

prosthesis, are "conformed" in correspondence with the joint site (e.g., by final shaping and curing processes that occur *in situ*).

Such conformation can also include aspects in which the components, or prosthesis itself, are adapted to be "deformed" within the site, as by the application of force. For instance, a substantially fully formed component can be provided to have sufficient mechanical properties (e.g., strength and resilience) to permit it to be inserted into a joint site and effectively deformed under normal anatomic forces. For instance, a substantially convex component can be deformed to assume the corresponding concave shape *in situ*, in , while retaining sufficient resilient strength to tend towards its original convex shape (e.g., analogous to the manner in which a locking washer can be deformed in use, while tending toward its original shape). Preferably, a final knee component is adapted to be deformed under conditions of use within the body (e.g., under physiologic load), while maintaining desired size and tibial congruency, and in a manner that provides desired fit and thickness for desired angular correction.

Hence a "preformed" component will generally refer to a component that is at least partially formed *ex vivo*, as by the surgeon's selection and use of an appropriately sized *ex vivo* mold. Such a preformed component can be specifically formed as well, including in an *ex vivo* fashion, as by the use of a customized mold that is itself reflective of the particular dimensions and contours of the intended joint site. Such customized molds can be prepared, for instance, by the use of external imaging means, and/or by the appropriate use of negative and/or positive molds taken at the tissue site. Optionally, and preferably, the preformed component is specifically formed, in whole or in part, by being positioned *in situ*, prior to the completion of the curing process, and in apposition to both supporting bone and opposing bone surfaces. Once positioned within the joint site, any such component or prosthesis can be adapted to be deformed

in order to improve its retention and/or performance *in situ*, e.g., resiliently deformed upon release of distracting forces and repositioning of the opposing bone surface.

For instance, a preformed composition is provided, formed initially by the *ex vivo* onset of cure, in which the composition can be implanted within on the order of 10 seconds to several days of the onset of cure, preferably within about 30 seconds to about 10 minutes, and more preferably within about one to about five minutes, while maintaining a surface exotherm of less than about 50C, and more preferably less than about 45C once positioned within the body.

Once positioned *in vivo*, preferred preformed components of this invention are adapted to be finally shaped, for a period of between about 10 seconds and one or more hours, and more preferably between about one minute and about five minutes. The lower limit is defined largely by the time it takes to effectively reposition bone, or otherwise re-establish suitable force on the implant. The upper limit, in turn, is generally defined by the susceptibility of the implanted composition to further deformation or shaping. Such final shaping is generally accomplished, at least in part, under the force brought about by repositioning articulating bone surfaces. In one preferred embodiment, the partially cured composition is implanted under conditions that permit it to deform less than about 15%, preferably less than about 10%, and most preferably less than about 5%, under physiologic forces, while maintaining tibial congruency and imparting desired angular correction.

Hence, a particularly preferred preformed component of this invention can be implanted within an initial about one to about five minutes of the onset of its formation, and once implanted can be further molded or formed for a further period of about one to about five additional minutes, in a manner that permits the resultant implant to substantially retain a desired final form and function.

1
2
3
4
5 The system of the present invention thereby provides the surgeon with a variety of options, based on the manner in which these curing and forming processes are correlated. In one particularly preferred embodiment, for instance, the surgeon is provided with a composition adapted to be partially cured and generally formed *ex vivo*, and then promptly inserted into the body and positioned at the joint site, where it can be finally, and specifically, formed in the course of becoming fully cured.

6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60
61
62
63
64
65
66
67
68
69
70
71
72
73
74
75
76
77
78
79
80
81
82
83
84
85
86
87
88
89
90
91
92
93
94
95
96
97
98
99
100
101
102
103
104
105
106
107
108
109
110
111
112
113
114
115
116
117
118
119
120
121
122
123
124
125
126
127
128
129
130
131
132
133
134
135
136
137
138
139
140
141
142
143
144
145
146
147
148
149
150
151
152
153
154
155
156
157
158
159
160
161
162
163
164
165
166
167
168
169
170
171
172
173
174
175
176
177
178
179
180
181
182
183
184
185
186
187
188
189
190
191
192
193
194
195
196
197
198
199
200
201
202
203
204
205
206
207
208
209
210
211
212
213
214
215
216
217
218
219
220
221
222
223
224
225
226
227
228
229
230
231
232
233
234
235
236
237
238
239
240
241
242
243
244
245
246
247
248
249
250
251
252
253
254
255
256
257
258
259
260
261
262
263
264
265
266
267
268
269
270
271
272
273
274
275
276
277
278
279
280
281
282
283
284
285
286
287
288
289
290
291
292
293
294
295
296
297
298
299
300
301
302
303
304
305
306
307
308
309
310
311
312
313
314
315
316
317
318
319
320
321
322
323
324
325
326
327
328
329
330
331
332
333
334
335
336
337
338
339
340
341
342
343
344
345
346
347
348
349
350
351
352
353
354
355
356
357
358
359
360
361
362
363
364
365
366
367
368
369
370
371
372
373
374
375
376
377
378
379
380
381
382
383
384
385
386
387
388
389
390
391
392
393
394
395
396
397
398
399
400
401
402
403
404
405
406
407
408
409
410
411
412
413
414
415
416
417
418
419
420
421
422
423
424
425
426
427
428
429
430
431
432
433
434
435
436
437
438
439
440
441
442
443
444
445
446
447
448
449
450
451
452
453
454
455
456
457
458
459
460
461
462
463
464
465
466
467
468
469
470
471
472
473
474
475
476
477
478
479
480
481
482
483
484
485
486
487
488
489
490
491
492
493
494
495
496
497
498
499
500
501
502
503
504
505
506
507
508
509
510
511
512
513
514
515
516
517
518
519
520
521
522
523
524
525
526
527
528
529
530
531
532
533
534
535
536
537
538
539
540
541
542
543
544
545
546
547
548
549
550
551
552
553
554
555
556
557
558
559
560
561
562
563
564
565
566
567
568
569
570
571
572
573
574
575
576
577
578
579
580
581
582
583
584
585
586
587
588
589
590
591
592
593
594
595
596
597
598
599
600
601
602
603
604
605
606
607
608
609
610
611
612
613
614
615
616
617
618
619
620
621
622
623
624
625
626
627
628
629
630
631
632
633
634
635
636
637
638
639
640
641
642
643
644
645
646
647
648
649
650
651
652
653
654
655
656
657
658
659
660
661
662
663
664
665
666
667
668
669
670
671
672
673
674
675
676
677
678
679
680
681
682
683
684
685
686
687
688
689
690
691
692
693
694
695
696
697
698
699
700
701
702
703
704
705
706
707
708
709
710
711
712
713
714
715
716
717
718
719
720
721
722
723
724
725
726
727
728
729
730
731
732
733
734
735
736
737
738
739
740
741
742
743
744
745
746
747
748
749
750
751
752
753
754
755
756
757
758
759
760
761
762
763
764
765
766
767
768
769
770
771
772
773
774
775
776
777
778
779
780
781
782
783
784
785
786
787
788
789
790
791
792
793
794
795
796
797
798
799
800
801
802
803
804
805
806
807
808
809
810
811
812
813
814
815
816
817
818
819
820
821
822
823
824
825
826
827
828
829
830
831
832
833
834
835
836
837
838
839
840
841
842
843
844
845
846
847
848
849
850
851
852
853
854
855
856
857
858
859
860
861
862
863
864
865
866
867
868
869
870
871
872
873
874
875
876
877
878
879
880
881
882
883
884
885
886
887
888
889
890
891
892
893
894
895
896
897
898
899
900
901
902
903
904
905
906
907
908
909
910
911
912
913
914
915
916
917
918
919
920
921
922
923
924
925
926
927
928
929
930
931
932
933
934
935
936
937
938
939
940
941
942
943
944
945
946
947
948
949
950
951
952
953
954
955
956
957
958
959
960
961
962
963
964
965
966
967
968
969
970
971
972
973
974
975
976
977
978
979
980
981
982
983
984
985
986
987
988
989
990
991
992
993
994
995
996
997
998
999
1000
1001
1002
1003
1004
1005
1006
1007
1008
1009
1010
1011
1012
1013
1014
1015
1016
1017
1018
1019
1020
1021
1022
1023
1024
1025
1026
1027
1028
1029
1030
1031
1032
1033
1034
1035
1036
1037
1038
1039
1040
1041
1042
1043
1044
1045
1046
1047
1048
1049
1050
1051
1052
1053
1054
1055
1056
1057
1058
1059
1060
1061
1062
1063
1064
1065
1066
1067
1068
1069
1070
1071
1072
1073
1074
1075
1076
1077
1078
1079
1080
1081
1082
1083
1084
1085
1086
1087
1088
1089
1090
1091
1092
1093
1094
1095
1096
1097
1098
1099
1100
1101
1102
1103
1104
1105
1106
1107
1108
1109
1110
1111
1112
1113
1114
1115
1116
1117
1118
1119
1120
1121
1122
1123
1124
1125
1126
1127
1128
1129
1130
1131
1132
1133
1134
1135
1136
1137
1138
1139
1140
1141
1142
1143
1144
1145
1146
1147
1148
1149
1150
1151
1152
1153
1154
1155
1156
1157
1158
1159
1160
1161
1162
1163
1164
1165
1166
1167
1168
1169
1170
1171
1172
1173
1174
1175
1176
1177
1178
1179
1180
1181
1182
1183
1184
1185
1186
1187
1188
1189
1190
1191
1192
1193
1194
1195
1196
1197
1198
1199
1200
1201
1202
1203
1204
1205
1206
1207
1208
1209
1210
1211
1212
1213
1214
1215
1216
1217
1218
1219
1220
1221
1222
1223
1224
1225
1226
1227
1228
1229
1230
1231
1232
1233
1234
1235
1236
1237
1238
1239
1240
1241
1242
1243
1244
1245
1246
1247
1248
1249
1250
1251
1252
1253
1254
1255
1256
1257
1258
1259
1260
1261
1262
1263
1264
1265
1266
1267
1268
1269
1270
1271
1272
1273
1274
1275
1276
1277
1278
1279
1280
1281
1282
1283
1284
1285
1286
1287
1288
1289
1290
1291
1292
1293
1294
1295
1296
1297
1298
1299
1300
1301
1302
1303
1304
1305
1306
1307
1308
1309
1310
1311
1312
1313
1314
1315
1316
1317
1318
1319
1320
1321
1322
1323
1324
1325
1326
1327
1328
1329
1330
1331
1332
1333
1334
1335
1336
1337
1338
1339
1340
1341
1342
1343
1344
1345
1346
1347
1348
1349
1350
1351
1352
1353
1354
1355
1356
1357
1358
1359
1360
1361
1362
1363
1364
1365
1366
1367
1368
1369
1370
1371
1372
1373
1374
1375
1376
1377
1378
1379
1380
1381
1382
1383
1384
1385
1386
1387
1388
1389
1390
1391
1392
1393
1394
1395
1396
1397
1398
1399
1400
1401
1402
1403
1404
1405
1406
1407
1408
1409
1410
1411
1412
1413
1414
1415
1416
1417
1418
1419
1420
1421
1422
1423
1424
1425
1426
1427
1428
1429
1430
1431
1432
1433
1434
1435
1436
1437
1438
1439
1440
1441
1442
1443
1444
1445
1446
1447
1448
1449
1450
1451
1452
1453
1454
1455
1456
1457
1458
1459
1460
1461
1462
1463
1464
1465
1466
1467
1468
1469
1470
1471
1472
1473
1474
1475
1476
1477
1478
1479
1480
1481
1482
1483
1484
1485
1486
1487
1488
1489
1490
1491
1492
1493
1494
1495
1496
1497
1498
1499
1500
1501
1502
1503
1504
1505
1506
1507
1508
1509
1510
1511
1512
1513
1514
1515
1516
1517
1518
1519
1520
1521
1522
1523
1524
1525
1526
1527
1528
1529
1530
1531
1532
1533
1534
1535
1536
1537
1538
1539
1540
1541
1542
1543
1544
1545
1546
1547
1548
1549
1550
1551
1552
1553
1554
1555
1556
1557
1558
1559
1560
1561
1562
1563
1564
1565
1566
1567
1568
1569
1570
1571
1572
1573
1574
1575
1576
1577
1578
1579
1580
1581
1582
1583
1584
1585
1586
1587
1588
1589
1590
1591
1592
1593
1594
1595
1596
1597
1598
1599
1600
1601
1602
1603
1604
1605
1606
1607
1608
1609
1610
1611
1612
1613
1614
1615
1616
1617
1618
1619
1620
1621
1622
1623
1624
1625
1626
1627
1628
1629
1630
1631
1632
1633
1634
1635
1636
1637
1638
1639
1640
1641
1642
1643
1644
1645
1646
1647
1648
1649
1650
1651
1652
1653
1654
1655
1656
1657
1658
1659
1660
1661
1662
1663
1664
1665
1666
1667
1668
1669
1670
1671
1672
1673
1674
1675
1676
1677
1678
1679
1680
1681
1682
1683
1684
1685
1686
1687
1688
1689
1690
1691
1692
1693
1694
1695
1696
1697
1698
1699
1700
1701
1702
1703
1704
1705
1706
1707
1708
1709
1710
1711
1712
1713
1714
1715
1716
1717
1718
1719
1720
1721
1722
1723
1724
1725
1726
1727
1728
1729
1730
1731
1732
1733
1734
1735
1736
1737
1738
1739
1740
1741
1742
1743
1744
1745
1746
1747
1748
1749
1750
1751
1752
1753
1754
1755
1756
1757
1758
1759
1760
1761
1762
1763
1764
1765
1766
1767
1768
1769
1770
1771
1772
1773
1774
1775
1776
1777
1778
1779
1780
1781
1782
1783
1784
1785
1786
1787
1788
1789
1790
1791
1792
1793
1794
1795
1796
1797
1798
1799
1800
1801
1802
1803
1804
1805
1806
1807
1808
1809
1810
1811
1812
1813
1814
1815
1816
1817
1818
1819
1820
1821
1822
1823
1824
1825
1826
1827
1828
1829
1830
1831
1832
1833
1834
1835
1836
1837
1838
1839
1840
1841
1842
1843
1844
1845
1846
1847
1848
1849
1850
1851
1852
1853
1854
1855
1856
1857
1858
1859
1860
1861
1862
1863
1864
1865
1866
1867
1868
1869
1870
1871
1872
1873
1874
1875
1876
1877
1878
1879
1880
1881
1882
1883
1884
1885
1886
1887
1888
1889
1890
1891
1892
1893
1894
1895
1896
1897
1898
1899
1900
1901
1902
1903
1904
1905
1906
1907
1908
1909
1910
1911
1912
1913
1914
1915
1916
1917
1918
1919
1920
1921
1922
1923
1924
1925
1926
1927
1928
1929
1930
1931
1932
1933
1934
1935
1936
1937
1938
1939
1940
1941
1942
1943
1944
1945
1946
1947
1948
1949
1950
1951
1952
1953
1954
1955
1956
1957
1958
1959
1960
1961
1962
1963
1964
1965
1966
1967
1968
1969
1970
1971
1972
1973
1974
1975
1976
1977
1978
1979
1980
1981
1982
1983
1984
1985
1986
1987
1988
1989
1990
1991
1992
1993
1994
1995
1996
1997
1998
1999
2000
2001
2002
2003
2004
2005
2006
2007
2008
2009
2010
2011
2012
2013
2014
2015
2016
2017
2018
2019
2020
2021
2022
2023
2024
2025
2026
2027
2028
2029
2030
2031
2032
2033
2034
2035
2036
2037
2038
2039
2040
2041
2042
2043
2044
2045
2046
2047
2048
2049
2050
2051
2052
2053
2054
2055
2056
2057
2058
2059
2060
2061
2062
2063
2064
2065
2066
2067
2068
2069
2070
2071
2072
2073
2074
2075
2076
2077
2078
2079
2080
2081
2082
2083
2084
2085
2086
2087
2088
2089
2090
2091
2092
2093
2094
2095
2096
2097
2098
2099
2100
2101
2102
2103
2104
2105
2106
2107
2108
2109
2110
2111
2112
2113
2114
2115
2116
2117
2118
2119
2120
2121
2122
2123
2124
2125
2126
2127
2128
2129
2130
2131
2132
2133
2134
2135
2136
2137
2138
2139
2140
2141
2142
2143
2144
2145
2146
2147
2148
2149
2150
2151
2152
2153
2154
2155
2156
2157
2158
2159
2160
2161
2162
2163
2164
2165
2166
2167
2168
2169
2170
2171
2172
2173
2174
2175
2176
2177
2178
2179
2180
2181
2182
2183
2184
2185
2186
2187
2188
2189
2190
2191
2192
2193
2194
2195
2196
2197
2198
2199
2200
2201
2202
2203
2204
2205
2206
2207
2208
2209
2210
2211
2212
2213
2214
2215
2216
2217
2218
2219
2220
2221
2222
2223
22

In addition to its immediate use in such joints as the knee, the system of the present invention provides particular advantages when applied to ball and socket joints, such as the hip. In one such embodiment, a balloon can be filled with a biomaterial as described herein, and inserted and positioned within the acetabulum, prior to or following filling, to provide a soft, conformable, durable lining for the placement of a hip prosthetic portion.

In a further embodiment, the method and system involve the preparation and use of one or more partially or fully cured component(s) formed outside the body, for insertion and placement into the body and optionally further fitting and securing at the joint site. These preformed component(s) typically require less manipulation at the bedside and allow for alternative methods of terminal sterilization, and final inspection and release at the manufacturing site.

DETAILED DESCRIPTION

The method and system (e.g., preformed component(s) and/or curable biomaterial and mold) can be used to prepare a final prosthesis, *in vivo*, that provides a first major surface in apposition to and retained upon the supporting bone itself, and a second (generally substantially parallel and opposite) major surface adapted to provide a wear surface for opposing (e.g., articulating) bone. By "retained upon" it is meant that the final prosthesis is maintained in a desired position upon the supporting bone surface in a manner suitable for its intended use, e.g., by the use of one or more anchor points, by the use of adhesive or other suitable interface materials, by the use of sutures, staples, and the like, and/or by a mechanical lock achieved by the combination of a bone-contacting surface suitably conformed or conformable to the terrain of

supporting bone, together with the retaining (and optionally including deforming) effect achieved upon repositioning opposing articulating bone surface.

The first and second major surfaces can be provided in any suitable manner, for instance,

1) by the preparation and insertion of a single partially cured and generally preformed component into the joint, preferably under conditions that permit the component to become further, and specifically, formed *in vivo*, 2) by adding a flowable biomaterial to an initial preformed component (e.g., in the shape of a balloon or open mold) positioned at the tissue site, 3) by placing one or more fully cured and preformed components at the tissue site and optionally further fitting, adapting and/or securing the component(s) as needed, and/or 4) by assembling one or more preformed components *in situ* (e.g., side by side in an interlocking fashion upon the surface) such that the assembled components cooperate to provide the first and second major surfaces.

In addition to the partially or fully cured preformed component(s) and/or curable biomaterial and related molds, the method and system of this invention include the optional use of various additional materials and/or steps, e.g., to prepare the bone surface itself, to provide suitable interfaces (e.g., adhesive interfaces and/or protrusions that can be further secured to the joint site or by smoothing of the femoral condyle or tibial plateau as needed), to treat one or more surfaces in order to provide them with different or improved properties as compared to the inherent properties of the material providing the surface, and the like. Examples of such materials include, for instance, the use of adhesive materials, tissue in-growth stimulators, and fibrous materials (e.g., webs adapted to tether the implant and/or to facilitate fibrous tissue ingrowth).

5 The partially or fully cured preformed component(s) can themselves each provide uniform or non-uniform properties, and can be provided in a plurality or range of styles and sizes. These components can be designed to conform to lateral or medial compartments, or both, and to right or left knees, or both. In a preferred embodiment, all embodiments can be inserted into the joint site in a minimally invasive fashion. By "minimally invasive", in this context, it is meant that the procedure of sizing, inserting, positioning and forming the prosthesis, *in situ*, can preferably be accomplished without the need for open, invasive incisions of the type conventionally used for inserting total knee prostheses. In a preferred embodiment, the partially cured preformed components can be further formed and fully cured *in vivo* to enhance compliance with the joint site.

20 The surface of the partially or fully cured preformed component(s) can also be modified to provide any desired properties (e.g., promote adhesion), such as by the design and use of polymers themselves or by surface treatment of the fully cured or curing embodiments to provide suitable reactive groups such as amines, hydroxyl groups, or other reactive or hydrogen bonding functionalities. Similarly, the partially cured preformed component or fully cured component, including balloons or composite materials, can be provided with appropriate surface coatings, e.g., biologically active agents to promote desired tissue interactions, including tissue or cellular adhesion, such as those selected from the group consisting of cytokines, hydroxyapatite, collagen, and combinations thereof.

20 In one embodiment of this invention, partially cured, and generally preformed components are inserted into the joint site, and there further and specifically formed to enhance compliance. In an alternative embodiment, fully cured components in the shape of a balloon or open mold are employed to provide a final composite material by inserting the balloon or mold

into the joint and there filling it with a biomaterial that cures *in situ* and conforms with the joint site. In another alternative embodiment, the fully cured component(s) are provided and inserted into the joint either singly or piecemeal and optionally further fitted and secured *in vivo*.

As an example of the first such embodiment, the invention provides an open *ex vivo* mold, adapted to approximate the desired dimensions of the joint site, and to receive a curable biomaterial. A suitable mold can be formed, for instance, from the use of conventional materials such as silicone materials, that permit the curing biomaterial component to be easily and entirely removed at the desired time. Optionally, the mold can itself be provided with a coating or release liner, including those that can be integrated, in whole or in part, with the component thus formed. Once the flowable biomaterial has been delivered and partially cured in this *ex vivo* mold, and any optional molding or fabricating steps have occurred, the biomaterial can be removed from the mold and inserted into the joint site, under conditions suitable to permit it to be further and finally formed *in vivo* to enhance conformance with the joint site. Optionally, additional *ex vivo* forming steps or features can be performed, e.g., by imparting desired curvature and femoral glide paths, prior to inserting and final forming *in vivo*.

Also, in the course of molding the component *ex vivo*, and/or transferring it to the tissue site, various structures and/or materials can be incorporated into and/or onto the component itself, to enhance its placement, retention and/or performance *in situ*. For instance, the mold itself can be provided in a form sufficient to impart various integral structural features, such as tibial "tabs", adapted to provide or improve the retention of the component at the tissue site. Such tabs, for instance, can be provided in the form of one or more protrusions integral with the mold itself and adapted to be positioned within and/or affixed to the soft tissue and/or bone *in*

vivo. Examples of such tabs are shown, for instance, in Figure 1, where reference number 18 depicts a raised posterior portion.

An insertable component can also be provided with one or more ancillary portions or protrusions formed of materials other than that used to form the bulk of the component itself.

5 For instance, sutures or fibrous materials can be incorporated into or onto the bulk material, for use in improving the initial and/or long term retention of the component *in situ*, e.g, by tethering the prosthesis at the joint site and in a desired position. Such other materials can be temporarily positioned into or upon the mold itself, for instance, or otherwise provided, in a manner that permits them to become integrated into the biomaterial as it fills the mold and becomes partially cured *ex vivo*. With the resulting component positioned *in situ*, the protrusions can be used to tether the implant, by securing them to the surrounding soft tissue and/or bone by use of adhesives, sutures, screws, pins, staples or the like or combinations thereof. The materials can provide both an immediate fixation function, and optionally also a desired long term function, by permitting them to be either absorbed by the body over time, and/or to permit or encourage fibrous tissue ingrowth for long term fixation.

The reinforcing material can be provided in any suitable form, e.g., as fibers (e.g., sutures) or as a uniform woven or non-woven fabric, optionally including one or more reinforcing fibers or layers. A suitable non-woven fabric, for instance, is preferably a material such as is commercially available under the trade name Trevira Spunbond from Hoechst

20 Celanese Corporation. The non-woven fabric is generally composed of continuous thermoplastic fiber, needle punched together to yield a felt-like fabric. In addition to fabrics like Trevira Spunbond, other materials such as polyester staple mat, glass fiber mat, as well as other organic and inorganic fiber mats and fabrics can be employed.

Reinforcing fibers can be included within the woven or non-woven fabric, or provided as separate layers of a composite. Such fiber layers can preferably include a directional reinforcing fiber layer of organic or inorganic structural reinforcing fibers such as fiberglass, carbon fibers, aramid fibers which is available from DuPont Corporation under the trade name Kevlar, linear polyethylene or polypropylene fibers such as is commercially available from Allied-Signal, Inc. (now Honeywell) under the trade name Spectra, or polyester fibers. The phrase "reinforcing fiber" can include any fiber which, when used in its own right or added to a composite fabric material, retains or enhances desired structural properties. The fibers can be randomly oriented, or preferentially, they can be oriented in one or more directions. While a number of specific types of materials have been given for use as the reinforcing fiber layer, it will be appreciated by those of ordinary skill in the art that other equivalent-type reinforcing fiber layers can be employed in the practice of the invention. A reinforcing fiber layer can be itself used to secure the prosthesis, or can be attached to a woven or non-woven fiber layer having a number of interstices or pores. Preferably, the reinforcing fiber layer and other fiber layers are secured to each other mechanically, as by conventional stitching, needle punching, stapling or buttons. In the case of certain applications, adhesives can also be used.

Similarly, a partially cured preformed component (and/or ancillary portions incorporated therein) can also be provided with suitable means to improve its ability to retain the component *in situ*, e.g., by the use of surface characteristics that provide improved chemical interactions with the joint site. Such interactions can be achieved by the judicious use of bulk material compositions themselves and/or the use of adhesives or other suitable interface materials. The partially cured, preformed, component can also be physically modified to increase its interactions with joint site, as by surface roughening, etching or cross-hatching, which would tend to provide

increased surface area, and in turn, improved mechanical retention. A partially cured, preformed, component can also be retained by external means that are otherwise secured to the surrounding bone and/or soft tissue by use of adhesives, sutures, screws, pins, staples or the like or combinations thereof. On the major surface opposing articulating bone, the partially cured preformed component can be provided with suitable means as well, intended to improve or alter either its compliance and/or interactions with the opposing bone surface.

In one particularly preferred embodiment, the system includes a partially cured preformed component that is first molded outside of the joint site and adapted to be delivered to a tissue site and there positioned in a fixed position. The mold can be of an open or closed configuration (and/or can involve a one- or multi-step molding process), adapted to preform one or both major surfaces, respectively. Once positioned, the partially cured component is adapted to be initially fit and positioned within the joint site, and to thereafter become better conformed to the specific dimensions and/or terrain (e.g., anatomic structure) of the joint site *in vivo*. Optionally, and preferably, the molds are designed to yield components that have optimum adhesion and conformance to the joint sites. The molds may also be heated during the *ex vivo* partial curing process to optimize component properties or to provide a component that is more formable *in vivo*.

In an alternative preferred embodiment, the method and system involve the preparation and use of one or more fully or partially cured component(s) formed outside the body, for insertion and placement into the body and optionally further fitting and securing at the joint site. In one embodiment, the invention provides a single preformed component that is inserted into the joint site and optionally further fitted or secured as needed. In another embodiment, the invention provides a plurality of preformed components, formed of the same or different

materials, and adapted to be delivered and positioned at the tissue site in a manner that provides a final composite. The components can be combined at the site in any suitable fashion, e.g., by providing a mechanical lock and/or by the use of interfacial materials such as adhesive layers. The components can be combined in any suitable fashion, e.g., as layers upon the bone, or as individual side-by-side components adapted to traverse the bone surface when combined. The use of preformed component(s) can require less manipulation at the bedside and allow for alternative methods of terminal sterilization, and final inspection and release at the manufacturing site. The various means of retaining partially cured preformed components, discussed herein, can be adapted to work with fully cured preformed components.

The method and system of this invention can be used for repairing a variety of mammalian joints, including human joints selected from the group consisting of the tibial plateau of the knee, the acetabulum of the hip, the glenoid of the shoulder, the acromion process of the shoulder, the acromio-clavicular joint of the shoulder, the distal tibial surface of the ankle, the radial head of the elbow, the distal radius of the forearm, the proximal phalanx surface of the great toe, the proximal metacarpal surface of the thumb, and the trapezium of the wrist.

Those portions or combinations of preformed component(s) that contact the bone surface are preferably adapted to physically conform closely to the prepared bone surface, e.g., to its macroscopic physical contours. Such conformation can be provided or enhanced in any suitable manner, e.g., 1) by providing a partially cured preformed component that is first made in an *ex vivo* mold and then adapted or modified to conform to the surface (e.g., by further forming *in vivo*), and/or 2) by use of a preformed balloon or composite mold material that is inserted into the joint site and filled with a flowable biomaterial that cures *in vivo* so that it conforms with the joint site and/or 3) by the use of fully cured preformed component(s) that has optimum geometry

for biomaterial compliance once placed in the joint site and/or 4) by the preparation and use of a suitable (e.g., thin) interface material between bone and preformed component (e.g., adhesive, filler, or cement material), and/or 5) by the use of physical restraining means, such as adhesives, pins, staples screws, sutures or the like that are attached to protrusions in the component itself or to an external means of securing it.

The method and system of this invention will be further described with reference to the Drawing, wherein

Figure 1 shows a top and side perspective of a preferred preformed knee implant (10) prepared using an *ex vivo* mold according to the present invention. The implant provides a first major surface (12) adapted to be positioned upon the tibial surface, and a generally planar second major surface (14) adapted to be positioned against the femoral condyle. In a typical embodiment, the second major surface, in turn, is preferably provided with a femoral glide path (16) to facilitate its performance *in situ*, in the form of a generally central oval depression about 1 mm to about 5mm deep at its lowest point (2 mm as shown) and about 30 mm to about 50 mm in length by 10 mm to 30 mm in width (40 mm by 20 mm as shown). Those skilled in the art, given the present description, will readily determine the actual dimensions for optimal use, in both absolute and relative terms, depending on such factors as the actual joint size and desired results (e.g., angular correction). As shown, the implant is also provided with a raised tibial projection (18), adapted to catch the posterior portion of the tibial plateau. The implant can have dimensions on the order of between about 40 to about 60 mm in the anterior-posterior dimension, between about 30 mm to about 40 mm in the medial-lateral dimension, and a maximum thickness (at the posterior lip of between about 10 mm and about 20 mm.

Figure 2 shows an embodiment in which a plurality of preformed components are adapted to be inserted and assembled *in situ* to provide the final implant (20). Figure 2a shows an embodiment, in which preformed components (22 through 25, respectively) are assembled in a side-by-side manner sequentially, and *in situ*, and upon the tibial surface. The matable preformed sections each provide at least a portion of the resultant bone-contacting surface and wear surface, as well as one or more portions adapted to provide a mechanical lock with one or more respective other portions. The mechanical lock can be achieved in any suitable manner, as by the provision of corresponding male and female portions, respectively. The portions can be mated, *in situ*, e.g., in a press fit or sliding manner, in order to attach the respective components. As can be seen in the raised perspective of the same embodiment, and Figure 2b, in the resultant assembly, the combined components cooperate to provide both a tibial bone-contacting surface (28) and a wear surface (26).

In the alternative embodiment of Figure 3, rather than being positioned in a side-by-side fashion across the bone surface (as in Figure 2), a final implant is provided using interlocking preformed components (shown in this case as portions 31 through 33, respectively) are instead provided in a form that permits them to be stacked upon each other, e.g., by layering or sliding them onto each other, and positioned upon the surface, *in situ*. The portions can be assembled in any suitable fashion, e.g., entirely on the tissue site, entirely *ex vivo*, or in varying combinations as desired. Optionally, and preferably, the generally planar portions are provided with corresponding matable portions, e.g., in the form of grooves and tabs to provide a sliding fit, or a depression and corresponding projection to provide either a press fit, snap fit, or other suitable fit sufficient to prevent lateral displacement to the extent desired. The resultant formed prosthetic implant can be provided with various features as described herein, including desired molded

portions adapted to provide better fit or performance. Top portion (31) is particularly well suited to provide a desirable wear surface, while one or more intermediate portions (as shown by element 32) are adapted to provide an optimal combination of such properties as thickness, cushioning, and angular correction. As shown the lowermost portion (33) is shown with a projection (34) adapted to be retained within a corresponding anchor hole or suitable depression formed into the bone itself. Figures 3b and 3c provide generally bottom and top views, respectively, showing the manner in which the portions can be combined in a layered fashion.

In the embodiment of Figure 3, preformed layers are shown having protrusions adapted to be positioned in a corresponding indentation within each underlying layer (or bone), in order to form a compact stack. In such an embodiment, the corresponding system will typically include at least two preformed components, including the initial, bone-contacting component, and final component providing the wear surface. The system can provide one or more intermediate layers, e.g., the number and/or selection of which can be used to provide a final desired height to the overall composite, and/or to provide differing properties (e.g., with respect to compressibility, resilience, tissue ingrowth), and/or to provide improved retention between the first and final components.

Figure 4a shows an embodiment in which a substantially open (saucer-shaped) mold (40) is inserted into the joint site, to be filled with a corresponding curable biomaterial *in situ*. The top (42) of the mold is open to receive biomaterial (not show), while the bottom (44) provides a lower major surface (46) adapted to contact bone and terminates in a filled protrusion (48) adapted to be positioned within a corresponding anchor point drilled in the bone itself. The anterior edge (50) of the cup is substantially perpendicular to the plane of the cup itself, while the

posterior edge (52) is tapered (and optionally raised) to accommodate the corresponding shape of the tibial spine.

As shown, and for use in an adult human, the *ex vivo* mold accommodates a predetermined volume of biomaterial of on the order of about 5 ml to about 15 ml. As a further advantage of this invention, the amount of biomaterial actually can be predetermined and controlled to correspond with the *ex vivo* mold volume. In addition the *ex vivo* molds are designed for optimum sizing and conformance to the joint site and MRI software may be used to chose best mold for joint site. Implant thickness and hence angular correction can be controlled in this way.

Figure 4b shows a bottom perspective view of the mold apparatus of Figure 4a, showing the filled protrusion (48). The posterior edge portion (and particularly the posterior mesial edge portion, as seen in the figure) can be seen as provided with a groove or indentation (54), again to accommodate the typical shape of the corresponding tibial spine. Overall, the mold can be seen as assuming a generally kidney-shaped configuration, adapted to correspond with the tibial surface. Such a mold can be provided in a plurality of sizes, and shapes, to be selected at the time of use to accommodate the particular patient's needs and surgeon's desires.

Figures 5a and 5b show the mold of Figure 4a being positioned upon a tibial surface (Fig. 5a), with the protrusion positioned within a corresponding anchor point, and (in Fig. 5b) with the tip of a biomaterial delivery cannula (56) positioned upon it, and with flowable biomaterial (58) being shown in the course of delivery.

Figure 6 shows a variety of alternative embodiments that include one or more preformed component. Fig. 6a shows a simple wedge shaped embodiment (60), in which the posterior portion (62) is significantly increased in size as compared to the anterior (64). Fig. 6b shows an

implant (66) molded to provide portions (here, layers) having differing wear characteristics, including a preformed top having improved wear as compared to the separately formed bottom portion (70). Fig. 6c, by comparison, shows a plurality of components (72) adapted to be positioned and assembled in situ at the time of surgery. These include an upper portion (74) having improved wear characteristics as compared to the others, a bottom portion (78) being suitably formed to the patient's geometry and desired angular correction, and one (or more) central portions (76) adapted to be positioned between the top and bottom portions to achieve desired properties such as overall thickness, angles, and/or physical chemical properties (such as moduli).

The embodiment of Figure 6d shows a single piece (80) as might be cut from preformed material at the time of surgery, while Figure 7 shows a variety of alternative means for anchoring a preformed component such as that shown in Fig. 6d. These include the use of a grout (82) or other suitable interface material as shown in Fig. 7a; the use of a separate external retaining device (84) as shown in Fig. 7b; the use of externally provided pins, screws, sutures, etc. as exemplified by elements (86) which generally traverse the body itself as in Fig. 7c; and the use of one or more anchor portions (88) positioned along one or more suitable surfaces as shown in Fig. 7d.

Figure 8 shows a further variety for anchoring or stabilizing a preformed portion by the use of ancillary portions and/or surface texture, including a roughened surface (90) as in Fig. 8a; or tabs (e.g., provided by fabric or suture like materials) as shown as elements 92 and 94 of Figs. 8b and 8c, respectively. In practice, the preformed components can benefit from any suitable combination of the various features and embodiments described or shown herein.

Figure 9 shows a variety of embodiments in a substantially closed (balloon like) mold is adapted to be inserted into the joint site and filled with a corresponding curable biomaterial, the mold itself providing a preformed articulating wear surface, including Fig. 9a which shows an inflatable balloon portion (96) that includes an integral preformed wear surface and portion (98), as well as a lumen (100) adapted to fill the inflatable portion with flowable biomaterial. Fig. 9b shows a corresponding balloon (102) though without a preformed portion, and including its biomaterial lumen (104). Although not shown, the balloon of this or any embodiment can include various interior and/or exterior surface coatings, and can have regions and/or layers having different desired physical-chemical properties (such as porosity). Fig. 9c shows a bi-compartmental closed balloon-like mold (106), wherein each compartment is adapted to conform to a respective medial or lateral tibial surface.

Figure 10 shows a mold adapted for use as an acetabular mold (110) in connection with the replacement of the articulating surface in a hip, when filled with biomaterial, the mold forming a concave portion adapted to retain a corresponding femoral head. The mold is shown providing a thin generally cup-shaped mold adapted to be filled in any suitable form (e.g., using a removable conduit (not shown) attached to the space between inner and outer sealed layers (116 and 114, respectively) forming the mold.

Figure 11 shows a patella-femoral joint form suitable for use in combination with the method and system of this invention. As shown in the views of 11a through 11c, the form includes a silicone or other suitable pad material (122) having aluminum or other suitable stay portions (124) and terminal handle or grasping portions (126). In use, with the knee at a generally 45 degree angle, the piece is formed to the femoral bone surface, with its form maintained by bending the aluminum stays. With anchor points cut into the femoral bone, if

desired, the form is held tight against the bone with the upper handle held away from bone to permit the delivery of curable biopolymer between the form and the bone. As polymer is placed onto the bone (and into any anchor points) the form is maintained for a time sufficient to suitably form the polymer, whereafter it can be removed.

5 As described in Applicant's co-pending US provisional application 60/228,444, the present application describes a method and system for the creation or modification of the wear surface using an implanted material fixed to the support structure of the original wear surface, to generally conform to the shape of the original surface in a mammal. A method or system where the end of the bony surface is a rotating, sliding or rolling surface, such as in the knee, finger, hip, toe, spine, wrist, elbow, shoulder, ankle, or TMJ joint. The implant will function:

- a) as a spacer,
- b) as an impact absorber
- c) as a surface with improved coefficient of friction (as compared to the diseased surface), and/or
- d) to increase the weight bearing area and improve congruency of the joint surface (as compared to the diseased condition).

The method and system of this invention can be applied to areas of aseptic necrosis, such as the nevecular bone in the wrist. The material to be implanted consists of a plurality of materials, such as polymers, including polyurethane, polyethylenes, polyureas, polyacrylates, 20 polyurethane acrylates, hydrogels, epoxies and/or hybrids of any of the above.

In an alternative embodiment, the surface can be provided by any of a series of metals, including titanium, stainless steel, cobalt chrome millithium alloys and tantalum. Other surface materials can include various ceramics and biologic polymers.

20540301-034502

The implantable material for the resurfacing can be formed ex vivo and/or in vivo as an injectable material that sets up to the molded shape. The methods for changing state from liquid to solid state include cooling or heating, the passage of time, which allows for a change of state, or a chemical reaction between different reactants. The reaction can be exothermic or endothermic. The set-up can be light activated or chemically catalyzed or it could be heat activated. Examples of such systems include flowable polymers of two or more components, light activated polymers, and polymers cured either by catalysts or by heat, including body heat. Molds can be used in the form of balloons, dams or retainers. They can be used in combination with the local anatomy to produce the desired shape and geometry. Molds can be of materials that are retained and becomes part of the implant or could be removed after curing of the biomaterial component.

In an alternative embodiment, the material would be semi-solid and could be shaped and then set up in vivo. This would allow for the minimally invasive application, either through an arthroscopic portal or through a small mini arthrotomy. As a further embodiment, the material could be synthesized ex vivo and then machined to fit using imaging to pre-determine the desired geometry and size of the implant. As a further alternative, a range of implant sizes could be provided and sizing could be accomplished during the procedure. An ex vivo mold could be fit using molding materials and the implant could be molded on site just prior to implantation.

Fixation methods for the implant would include biologic glues to glue the implant to the underlying surface, trapping of the implant into a cavity on the surface that causes a mechanical lock, using various anchors to the underlying structure and fixing the implant to that surface or using mold retainers and/or screws, staples, sutures or pins. In alternative embodiment, anchors

in the underlying structure may be used for fixing the implant to that surface and we may also use a tissue ingrowth system to secure anchoring.

In the preferred embodiment, the patient will have a diagnosis of osteoarthritis and have loss of cartilage on the articulating surface. A determination will be made of the amount of correction needed for the reestablishment of a normal angle of articulation. The ligaments will be balanced so that there is no loss of range of motion with the implant in place and the surface will be placed in such a position that the eventual resulting surface geometry reestablishes the same plane and orientation of the original articular surface.

Access to the site is obtained in a minimally invasive way. In a preferred embodiment, this is accomplished through arthroscopic means with arthroscopic portals. In an alternative embodiment, the access is accomplished by a mini arthrotomy with a small incision that allows access to the joint without sacrificing nerves, vessels, muscles or ligaments surrounding the joint. In the preferred embodiment fibrillated articulating cartilage that is degenerated is removed down to the subchondral surface. The surface is dried and prepared for appropriate anchoring. This may include anchor points that give a mechanical lock or that alternatively simply supply horizontal and lateral stability. The surface may be prepared by drying and roughening in case a tissue adhesive is used. Pre-made anchors may be installed. These may be made of various metallic materials or of polymers and may consist of pegs that would extend up through the implant to anchor it to the underlying surface. This surrounding subchondral bone may be roughened to enhance tissue ingrowth or implant adhesion. The final geometry of the implant may be determined by a dam or mold that is placed on the joint at the time the material is implanted, when the implant is installed using an *in situ* cured technique (in the manner shown in Figures 1 and 4 of Applicant's provisional parent application).

For pre-made material formed at the surgical site within a mold, various forms of stabilization could be used, including anchor points or titanium screws. Alternatively, the pre-made material could be made off site to the specs developed from imaging of the patient's joint surface. In a third embodiment, multiple sizes could be made off site and the selection of the appropriate implant size could be chosen at the time of surgery. Two alternatives shown in Figure 2 of the parent provisional application include a single segment that can be installed through a portal or a series of segments that can be installed through a portal and locked together once inside the joint. They would be placed sequentially and then anchored to the bone by anchor points cut in the bone or by screws or tissue ingrowth. Finally, a robot, a jag or other cutting fixture could be used to prepare the bony surface for the pre-made implant to a fixed geometry of the anchor point.

Both the preformed component(s) and flowable biomaterial, if used, can be prepared from any suitable material. Typically, the materials include polymeric materials, having an optimal combination of such properties as biocompatibility, physical strength and durability, and compatibility with other components (and/or biomaterials) used in the assembly of a final composite. Examples of suitable materials for use in preparing the preformed component(s) may be the same or different from the *in situ* curing biomaterial, and include polyurethanes, polyethylenes, polypropylenes, Dacrons, polyureas, hydrogels, metals, ceramics, epoxies, polysiloxanes, polyacrylates, as well as biopolymers, such as collagen or collagen-based materials or the like and combinations thereof.

Examples of suitable materials for use in preparing the flowable biomaterial, if used, include polyurethanes, polyureas, hydrogels, epoxies, polysiloxanes, polyacrylates, and combinations thereof.

In a presently preferred embodiment, the preformed component(s) and the flowable biomaterial, if included, each comprise a biocompatible polyurethane. The same or different polyurethane formulations can be used to form both the preformed component(s), e.g., by an injection molding technique, as well as for the flowable biomaterial, if present.

5 Suitable polyurethanes for use as either the preformed component or biomaterial can be prepared by combining: (1) a quasi-prepolymer component comprising the reaction product of one or more polyols, and one or more diisocyanates, and optionally, one or more hydrophobic additives, and (2) a curative component comprising one or more polyols, one or more chain extenders, one or more catalysts, and optionally, other ingredients such as an antioxidant, and hydrophobic additive.

10098601.031502
205520-10986001

 In the embodiment in which an *in situ* curing polymer is used, the present invention preferably provides a biomaterial in the form of a curable polyurethane composition comprising a plurality of parts capable of being mixed at the time of use in order to provide a flowable composition and initiate cure, the parts including: (1) a quasi-prepolymer component comprising the reaction product of one or more polyols, and one or more diisocyanates, optionally, one or more hydrophobic additives, and (2) a curative component comprising one or more polyols, one or more chain extenders, one or more catalysts, and optionally, other ingredients such as an antioxidant, hydrophobic additive and dye. Upon mixing, the composition is sufficiently flowable to permit it to be delivered to the body, and there be fully cured under physiological

20 conditions. Preferably, the component parts are themselves flowable, or can be rendered flowable, in order to facilitate their mixing and use.

 The flowable biomaterial used in this invention preferably includes polyurethane prepolymer components that react either *ex vivo* or *in situ* to form solid polyurethane ("PU").

30093601-034502
The formed PU, in turn, includes both hard and soft segments. The hard segments are typically comprised of stiffer oligourethane units formed from diisocyanate and chain extender, while the soft segments are typically comprised of one or more flexible polyol units. These two types of segments will generally phase separate to form hard and soft segment domains, since they tend to be incompatible with one another. Those skilled in the relevant art, given the present teaching, will appreciate the manner in which the relative amounts of the hard and soft segments in the formed polyurethane, as well as the degree of phase segregation, can have a significant impact on the final physical and mechanical properties of the polymer. Those skilled in the art will, in turn, appreciate the manner in which such polymer compositions can be manipulated to produce cured and curing polymers with desired combination of properties within the scope of this invention.

The hard segments of the polymer can be formed by a reaction between the diisocyanate or multifunctional isocyanate and chain extender. Some examples of suitable isocyanates for preparation of the hard segment of this invention include aromatic diisocyanates and their polymeric form or mixtures of isomers or combinations thereof, such as toluene diisocyanates, naphthalene diisocyanates, phenylene diisocyanates, xylylene diisocyanates, and diphenylmethane diisocyanates, and other aromatic polyisocyanates known in the art. Other examples of suitable polyisocyanates for preparation of the hard segment of this invention include aliphatic and cycloaliphatic isocyanates and their polymers or mixtures or combinations thereof, such as cyclohexane diisocyanates, cyclohexyl-bis methylene diisocyanates, isophorone diisocyanates and hexamethylene diisocyanates and other aliphatic polyisocyanates. Combinations of aromatic and aliphatic or arylakyl diisocyanates can also be used.

10095601-0345007

The isocyanate component can be provided in any suitable form, examples of which include 2,4'-diphenylmethane diisocyanate, 4,4'-diphenylmethane diisocyanate, and mixtures or combinations of these isomers, optionally together with small quantities of 2,2'-diphenylmethane diisocyanate (typical of commercially available diphenylmethane diisocyanates). Other examples include aromatic polyisocyanates and their mixtures or combinations, such as are derived from phosgenation of the condensation product of aniline and formaldehyde. It is suitable to use an isocyanate that has low volatility, such as diphenylmethane diisocyanate, rather than more volatile materials such as toluene diisocyanate. An example of a particularly suitable isocyanate component is the 4,4'-diphenylmethane diisocyanate ("MDI"). Alternatively, it can be provided in liquid form as a combination of 2,2'-, 2,4'- and 4,4'- isomers of MDI. In a preferred embodiment, the isocyanate is MDI and even more preferably 4,4'-diphenylmethane diisocyanate.

Some examples of chain extenders for preparation of the hard segment of this invention include, but are not limited, to short chain diols or triols and their mixtures or combinations thereof, such as 1,4-butane diol, 2-methyl-1,3-propane diol, 1,3-propane-diol ethylene glycol, diethylene glycol, glycerol, cyclohexane dimethanol, triethanol amine, and methyldiethanol amine. Other examples of chain extenders for preparation of the hard segment of this invention include, but are not limited to, short chain diamines and their mixtures or combinations thereof, such as dianiline, toluene diamine, cyclohexyl diamine, and other short chain diamines known in the art.

The soft segment consists of urethane terminated polyol moieties, which are formed by a reaction between the polyisocyanate or diisocyanate or polymeric diisocyanate and polyol. Examples of suitable diisocyanates are denoted above. Some examples of polyols for

preparation of the soft segment of this invention include but are not limited to polyalkylene oxide ethers derived from the condensation of alkylene oxides (e.g. ethylene oxide, propylene oxide, and blends thereof), as well as tetrahydrofuran based polytetramethylene ether glycols, polycaprolactone diols, polycarbonate diols and polyester diols and combinations thereof. In a preferred embodiment, the polyols are polytetrahydrofuran polyols ("PTHF"), also known as polytetramethylene oxide ("PTMO") or polytetramethylene ether glycols ("PTMEG"). Even more preferably, the use of two or more of PTMO diols with different molecular weights selected from the commercially available group consisting of 250, 650, 1000, 1400, 1800, 2000 and 2900.

Two or more PTMO diols of different molecular weight can be used as a blend or separately, and in an independent fashion as between the different parts of the two part system. The solidification temperature(s) of PTMO diols is generally proportional to their molecular weights. The compatibility of the PTMO diols with such chain extenders as 1,4-butanediol is generally in the reverse proportion to molecular weight of the diol(s). Therefore the incorporation of the low molecular weight PTMO diols in the "curative" (part B) component, and higher molecular weight PTMO diols in the prepolymer (part A) component, can provide a two-part system that can be used at relatively low temperature. In turn, good compatibility of the low molecular weight PTMO diols with such chain extenders as 1,4-butanediol permits the preparation of two part systems with higher (prepolymer to curative) volume ratio. Amine terminated polyethers and/or polycarbonate-based diols can also be used for building of the soft segment.

The PU can be chemically crosslinked, e.g., by the addition of multifunctional or branched OH-terminated crosslinking agents or chain extenders, or multifunctional isocyanates.

Some examples of suitable crosslinking agents include, but are not limited to, trimethylol propane ("TMP"), glycerol, hydroxyl terminated polybutadienes, hydroxyl terminated polybutadienes (HOPB), trimer alcohols, Castor oil polyethyleneoxide (PEO), polypropyleneoxide (PPO) and PEO-PPO triols. In a preferred embodiment, HOPB is used as the crosslinking agent.

This chemical crosslinking augments the physical or "virtual" crosslinking of the polymer by hard segment domains that are in the glassy state at the temperature of the application. The optimal level of chemical cross-linking improves the compression set of the material, reduces the amount of the extractable components, and improves the biodegradability of the PU. This can be particularly useful in relatively soft polyurethanes, such as those suitable for the repair of damaged cartilage. Reinforcement by virtual cross-links alone may not generate sufficient strength for *in vivo* performance in certain applications. Additional cross-linking from the soft segment, potentially generated by the use of higher functional polyols can be used to provide stiffer and less elastomeric materials. In this manner a balancing of hard and soft segments, and their relative contributions to overall properties can be achieved.

Additionally, a polymer system of the present invention preferably contains at least one or more, biocompatible catalysts that can assist in controlling the curing process, including the following periods: (1) the induction period, and (2) the curing period of the biomaterial. Together these two periods, including their absolute and relative lengths, and the rate of acceleration or cure within each period, determines the cure kinetics or profile for the composition. Some examples of suitable catalysts for preparation of the formed PU of this invention include, but are not limited to, tin and tertiary amine compounds or combinations thereof such as dibutyl tin dilaurate, and tin or mixed tin catalysts including those available under the tradenames "Cotin

222", "Formrez UL-22" (Witco), "dabco" (a triethylene diamine from Sigma-Aldrich), stannous octanoate, trimethyl amine, and triethyl amine. In a preferred embodiment, the catalyst is Formrez UL-22 (Witco). In an alternative preferred embodiment, the catalyst is a combination Cotin 222 (CasChem) and dabco (Sigma-Aldrich).

5 The *in vivo* and *ex vivo* cured polyurethanes of this invention can be formed by the reaction of two parts. Part I of which (alternatively referred to as Part A) includes a di- or multifunctional isocyanate or quasi-prepolymer which is the reaction product of one or more OH-terminated components, and one or more isocyanates. Part II of the polyurethane (alternatively referred to as Part B herein) is a curative component that includes of one or more chain extenders and one or more polyols, and one or more catalysts, and other additives such as antioxidants and dyes. For a suitable formed PU, the stoichiometry between Parts I (quasi-prepolymer) and II (curative component), expressed in terms of NCO:OH molar ratio of the isocyanate terminated pre-polymer (Part I) and the curative component (Part II) is preferably within the range of about 0.8 to 1.0 to 1.2 to 1.0, and more preferably from about 0.9 to 1 to about 1.1 to 1.0.

Optionally, a reactive polymer additive can be included and is selected from the group consisting of hydroxyl- or amine-terminated compounds selected from the group consisting of polybutadiene, polyisoprene, polyisobutylene, silicones, polyethylene-propylenediene, copolymers of butadiene with acrylonitrile, copolymers of butadiene with styrene, copolymers of
20 isoprene with acrylonitrile, copolymers of isoprene with styrene, and mixtures of the above.

Suitable compositions for use in the present invention are those polymeric materials that provide an optimal combination of properties relating to their manufacture, application, and *in vivo* use. In the uncured state, such properties include component miscibility or compatibility,

processability, and the ability to be adequately sterilized or aseptically processed and stored. In the course of applying such compositions, suitable materials exhibit an optimal combination of such properties as flowability, moldability, and *in vivo* curability. In the cured state, suitable compositions exhibit an optimal combination of such properties as strength (e.g., tensile and compressive), modulus, biocompatibility and biostability.

When cured, the compositions demonstrate an optimal combination of properties, particularly in terms of their conformational stability and retention of physical shape, dissolution stability, biocompatibility, and physical performance, as well mechanical properties such as load-bearing strength, tensile strength, shear strength, shear fatigue resistance, impact absorption, wear resistance, and surface abrasion resistance. Such performance can be evaluated using procedures commonly accepted for the evaluation of natural tissue and joints, as well as the evaluation of materials and polymers in general. In particular, a preferred composition, in its cured form, exhibits mechanical properties that approximate or exceed those of the natural tissue it is intended to provide or replace.

To achieve these desirable uncured and delivery properties, a "polymer system", as used herein refers to the component or components used to prepare a polymeric composition of the present invention. In a preferred embodiment, a polymer system comprises the components necessary to form two parts: Part I being an NCO terminated pre-polymer (optionally referred to as an "isocyanate quasi-polymer"). The quasi-polymer of Part I typically includes a polyol component, optionally in combination with a hydrophobic additive component, and an excess of an isocyanate component. Part II of the two component system can include one long-chain polyols, chain extenders and/or cross-linkers, together with other ingredients (e.g., catalysts, stabilizers, plasticizers, antioxidants, dyes and the like). Such adjuvants or ingredients can be

added to or combined with any other component thereof either prior to or at the time of mixing, delivery, and/or curing.

In a particularly preferred embodiment, a polymer system of this invention is provided as a plurality of component parts and employs one or more catalysts. The component parts, including catalyst, can be mixed to initiate cure, and then delivered, set and fully cured under conditions (e.g., time and exotherm) sufficient for its desired purpose. Upon the completion of cure, the resultant composition provides an optimal combination of properties for use in repairing or replacing injured or damaged tissue. In a particularly preferred embodiment, the formulation provides an optimal combination of such properties as compatibility and stability of the biomaterial parts, ex vivo or *in situ* cure capability and characteristics (e.g., extractable levels, biocompatibility, thermal/ mechanical properties), mechanical properties (e.g., tensile, tear and fatigue properties), and biostability.

The volume ratio of the parts can also be used to improve and affect the uncured and curing properties. Compositions having two or more parts, are preferred. Where two parts are used, the relative volumes can range, for instance, from 1:10 to 10:1 (quasi-prepolymer to curative components, based on volume). A presently preferred range is between 2:1 and 1:2. As those skilled in the art will appreciate, given the present description, the optimal volume ratio is largely determined by the compatibility and the stability of part A and B.

In choosing an optimal volume ratio for a given formulation, those skilled in the art, given the present description, will appreciate the manner in which the following considerations can be addressed. The viscosity of the reactive parts, at the temperature used for either injection-molding preformed components, or for *in situ* cure, should provide an acceptable degree of

190098601-031502
mixing and flow rate, without causing mechanical failure of any component of the delivery system including cartridge, static mixer, gun and other components.

5 Preferably, the biomaterial is sufficiently flowable to permit it to be delivered (e.g., injected) into the mold or tissue site. The composition of both reactive parts must be such that these parts are homogeneous and phase stable in the temperature range of the application. Generally, the maximum temperature of the reaction exotherm is proportional to the concentration of the reactive groups in the mixed polymer. A high concentration of the reactive groups might evolve too high reaction exothermal energy and therefore cause thermal damage to the surrounding tissues. The reactive parts will preferably remain substantially liquid in form during mixing.

A desired and stable volume ratio of the components can be achieved in any suitable manner, e.g., by the use of dual-compartment cartridges with constant volume ratio or by using the injectors with delivery rates independently variable for each component.

Compatibility of the composition can also be affected (and improved) in other ways as well, e.g., by pre-heating the components prior to polymer application. To enhance the homogeneity of the components, the components of a preferred composition of this invention are preferably preheated before mixing and delivery, e.g., by heating to about 60 C to about 80 C for about 2 to about 6 hours prior to use. Preferably, the composition parts are cooled back to about 35 C to 37 C before use in injection.

20 Fully cured polymeric (e.g., polyurethane) biomaterials suitable for use in forming components of this invention provide an optimal combination of such properties as creep and abrasion resistance. Preferably, for instance, the biomaterial provides DIN abrasion values of less than about 100 mm³, more preferably less than about 80 mm³ and most preferably less than

about 60 mm³, as determined by ASTM Test Method D5963-96 ("Standard Test Method for Rubber Property Abrasion Resistance Rotary Drum Abrader").

10098604.031502
205TE0" F098600T

CLAIMS

What is claimed is:

1. A system for the creation or modification of the wear surface of an orthopedic
5 joint within a mammalian body, the system comprising one or more partially or fully preformed polymeric components, adapted to be inserted and positioned at a joint site to provide an implant having at least one major surface in apposition to supporting bone, and at least a second major surface in apposition to opposing bone.
2. A system according to claim 1 wherein one or more of the polymeric components are formed at the time of use, by the use of a curable polymer system adapted to be at least partially cured and partially formed by *ex vivo* molding in order to provide an implantable component adapted to be inserted and positioned *in vivo*, under conditions suitable to permit the implanted component to become finally formed upon reestablishing the natural joint space and in conformance with the opposing bone surfaces of the orthopedic joint site.
3. A system according to claim 1 wherein the polymeric components comprise a plurality of packaged, preformed components adapted to be assembled at the orthopedic joint site in a minimally invasive fashion to provide a final prosthesis having surfaces in conformance with the opposing bone surfaces of the orthopedic joint site.
4. A system according to claim 1 further comprising an *ex vivo* mold having a
20 molding surface adapted to provide a roughened, patterned, and/or contoured surface to the partially preformed component, in a manner sufficient to provide improved retention and fit of the component at the joint site.

5. A system according to claim 4 wherein the mold further provides ancillary means adapted to be incorporated into the preformed component for securing the component once formed in the joint site.

6. A system according to claim 5 wherein the ancillary means comprise one or more protrusions adapted to be attached to either soft tissue and/or bone at the joint site to improve fixation.

7. A system according to claim 4 wherein the contoured surface comprises a contour having one or more protrusions, integral with the preformed component, and formed during the *ex vivo* molding process.

8. A system according to claim 6 wherein the protrusions are adapted to be integrated into the preformed component during the *ex vivo* molding process.

9. A system according to claim 7 wherein the protrusions are comprised of sutures and/or fibrous biomaterials integrally formed with the component itself.

10. A system according to claim 4 further comprising separate means, not associated with the mold itself, for securing the component to the joint site, selected from the group consisting of adhesives, sutures, pins, staples, screws, and combinations thereof.

11. A system according to claim 1 wherein the one or more preformed polymeric component(s) are adapted to be inserted into a joint in a minimally invasive fashion.

12. A system according to claim 2 in which the preformed component(s) and/or corresponding mold(s) are provided in a plurality or range of styles and sizes for selection and use in the surgical field.

13. A system according to claim 1 wherein the implant is adapted for use on the tibial surface of the knee, and provides portions adapted to conform to the shape of the femoral condyle and corresponding medial tibial plateau, lateral tibial plateau, or both.

14. A system according to claim 1 wherein the polymeric component is fabricated from a material selected from the group consisting of polyurethanes, polyureas, hydrogels, polysiloxanes, polyacrylates, and epoxies, and combinations thereof.

15. A system according to claim 14 wherein the polymeric component comprises a polyurethane.

16. A system according to claim 15 wherein the polyurethane is prepared from polyisocyanate(s), short and long chain polyols, and optionally including one or more ingredients selected from the group hydrophobic additive(s), tin and/or amine catalyst(s), and antioxidant(s).

17. A system according to claim 16 wherein the polyurethane comprises aromatic polyisocyanates, PTMO's, and short chain diols.

18. A system according to claim 16 wherein the hydrophobic additive comprises hydroxyl-terminated polybutadiene, and the tin and/or amine catalyst(s) are adapted to promote the isocyanate - hydroxyl reaction preferentially and are selected from the group consisting of UL22, Cotin 222, 1,4-diazabicyclo[2.2.2]octane (dabco), and dibutyltin dilaurate (DBTDL), and combinations thereof.

19. A system according to claim 14, wherein the preformed polymeric component comprises one or more surfaces having attached thereto a biologically active agent selected from the group cytokines, growth factors, autologous growth factors, hydroxyapatite, collagen, and combinations thereof.

20. A system according to claim 14 wherein the surface of the preformed component is provided or modified with reactive groups to promote tissue adhesion.

21. A system according to claim 20 wherein the reactive groups are provided by the polymers used to fabricate the polymeric component, and are selected from amines, hydroxyl groups, or other reactive or hydrogen bonding functionalities.

22. A system for the creation or modification of the wear surface of an orthopedic joint within a mammalian body, the system comprising one or more preformed polymeric components adapted to be positioned within the joint site and one or more flowable biomaterial polymer compositions adapted to be arthroscopically injected into contact with a preformed component and cured *in situ* at the joint site in order to provide a composite implant.

23. A system according to claim 22 wherein the preformed polymeric components comprise an inflatable balloon having a preformed top weight-bearing wear portion and a preformed bottom portion adapted to conform to the shape of supporting bone.

24. A system according to claim 23 wherein the one or more portions of the balloon are fabricated from a natural or synthetic fabric adapted to permit tissue in-growth, and sufficiently permeable to permit air to escape while retaining the curable biomaterial.

25. A system according to claim 24 wherein the fabric is of sufficient permeability to permit physical interpenetration of the flowable polymer.

26. A system according to claim 23 wherein the bottom and/or top portions comprise materials selected from polyurethanes, polyethylenes, polypropylenes, metals, ceramics, biopolymers or the like and combinations thereof.

27. A system according to claim 23 wherein the top and bottom portions are provided with forms corresponding to the shape of a femoral condyle and tibial plateau, respectively.

28. A system according to claim 23 wherein the balloon further comprises a port adapted to fill the balloon with flowable biomaterial *in situ*, in a manner sufficient to force the top portion toward corresponding bone.

29. A system according to claim 23 wherein the bottom portion provides a raised protrusion sufficient to improve retention within the joint site and/or to provide a site for suturing, stapling, pinning, or screwing the portion within the joint site.

30. A system according to claim 22 wherein separate means are provided for securing the preformed component within the joint site.

31. A system according to claim 22, further comprising one or more biologically active agents adapted to be provided on one or more surfaces of the resultant composite implant.

32. A system according to claim 22 wherein the surface of the preformed component and/or resultant composite material are provided or modified with reactive groups to promote adhesion.

33. A system according to claim 32 wherein the reactive groups are either provided by the preformed component itself, or are separately added by suitable surface treatment of the component or resultant composite, and the reactive groups are selected from amines, hydroxyl groups, or other reactive or hydrogen bonding functionalities.

34. A system according to claim 22 in which one or more of the preformed components are provided in a plurality or range of styles and sizes.

35. A system according to claim 22 wherein the one or more flowable biomaterial(s) are adapted to be inserted into a joint using minimally invasive means.

36. A system for the creation or modification of the wear surface of an orthopedic joint within a mammalian body, the system comprising a plurality of packaged, preformed

components adapted to be assembled at the orthopedic joint site in a minimally invasive fashion to provide a final prosthesis having surfaces in apposition to and conformance with the opposing bone surfaces of the orthopedic joint site.

37. A system according to claim 36 wherein one or more of the preformed components are provided with surfaces suitably roughened, patterned, or contoured to provide maximum adhesion and fit when placed, and optionally further fitted and secured, within the joint site.

38. A system according to claim 36, wherein one or more of the preformed components are formed at the time of use by the use of a curable biomaterial adapted to completely cure when preformed and then placed and optionally further fitted or secured inside the joint site.

39. A system according to claim 36 wherein one or more of the preformed components provide means for further securing the component once placed in the joint site.

40. A system according to claim 39 wherein the retention means to secure the component includes the use of tissue adhesives to improve fixation.

41. A system according to claim 39 wherein the retention means comprise one or more protrusions adapted to be sutured, pinned, stapled, screwed or combinations thereof or otherwise mechanically attached into the surrounding soft tissue and/or bone to improve fixation.

42. A system according to claim 41 wherein the protrusions are themselves integral with the preformed component.

43. A system according to claim 42 wherein the protrusions are integrated into a flowable biomaterial during the *ex vivo* molding process used to form the preformed component.

44. A system according to claim 43 wherein the protrusions are comprised of sutures or fibrous materials.

45. A system according to claim 39 wherein means to secure the component are external to it and secured once inside the joint site by the use of adhesives, sutures, pins, staples, screws or the like and combinations thereof to improve fixation to the surrounding soft tissue and/or bone to improve fixation.

46. A system according to claim 36 wherein the one or more preformed component(s) are adapted to be inserted into a joint in a minimally invasive fashion.

47. A system according to claim 36 in which the one or more preformed component(s) are provided in a plurality or range of styles and sizes.

48. A system according to claim 37 wherein the assembled components conform to the shape of the femoral condyle and tibial plateau, medial, lateral or both.

49. A system according to claim 37 wherein the preformed component(s) are fabricated from materials selected from the group consisting of polyurethanes, polyethylenes, polyureas, hydrogels, polysiloxanes, polyacrylates, epoxies, and combinations thereof.

50. A system according to claim 49 wherein the material comprises a polyurethane.

51. A system according to claim 50 wherein polyurethane is prepared from polyisocyanate(s), short and long chain polyols, and optionally including one or more ingredients selected from the group hydrophobic additive(s), tin and/or amine catalyst(s), and antioxidant(s).

52. A system according to claim 51 wherein the polyurethanes are prepared from aromatic polyisocyanates, PTMO's, short chain diols.

53. A system according to claim 52 wherein the hydrophobic additive comprises hydroxyl-terminated polybutadiene, and the tin and/or amine catalyst(s) used promote the

isocyanate - hydroxyl reaction preferentially and are selected from the group consisting of UL22, Cotin 222, 1,4-diazabicyclo[2.2.2]octane (dabco), and dibutyltin dilaurate (DBTDL) or the like and combinations thereof.

54. A system according to claim 36 wherein the preformed components provide one or more surfaces having attached thereto a biologically active agent selected from the group cytokines, hydroxyapatite, growth factors, autologous growth factors, collagen or the like and combinations thereof.

55. A system according to claim 36 wherein the surface of one or more preformed component(s) is provided or modified with reactive groups to promote tissue adhesion.

56. A system according to claim 55 wherein the reactive groups are covalently attached to the polymers used to fabricate the preformed component(s), and are selected from amines, hydroxyl groups, or other reactive or hydrogen bonding functionalities.

57. A system according to claim 36 wherein the preformed component(s) are selected from the group consisting of a) a single preformed component, b) a plurality of components adapted to be layered upon each other at the tissue site, c) a plurality of components adapted to be assembled at the tissue site in an interlocking fashion, such that the components cooperate to provide a respective portion of the first and second major surfaces.

58. A system according to claims 1 or 22 or 36 further comprising the use of one or more additional materials and/or steps adapted to a) prepare the bone surface itself, b) provide a desired interface between bone, component(s), and/or the physiologic environment, and/or c) treat one or more surfaces of the component(s) in order to provide them with different or improved properties as compared to the inherent properties of the material providing the surface.

59. A system according to claim 58 wherein the materials and/or steps are adapted to affect, improve or provide a surface property or function selected from adhesion, lubricity, smoothness, conformance, tissue in-growth, or biocompatibility.

60. A system according to claims 1 or 22 or 36 wherein the system is adapted to be used for repairing a variety of mammalian joints, including human joints selected from the group consisting of the tibial plateau of the knee, the acetabulum of the hip, the glenoid of the shoulder, the acromion process of the shoulder, the acromio-clavicular joint of the shoulder, the distal tibial surface of the ankle, the radial head of the elbow, the distal radius of the forearm, the proximal phalanx surface of the great toe, the proximal metacarpal surface of the thumb, and the trapezium of the wrist.

61. A system according to claim 60 wherein the system is adapted to be used for repairing the tibial plateau of the knee.

62. A system according to claim 60 wherein the system is adapted to be used for repairing the acetabulum of the hip.

63. A system according to claim 13 wherein the implant is provided in the form of a preformed knee implant prepared using an *ex vivo* mold and having a first major surface adapted to be positioned upon the tibial surface, and a second major surface adapted to be positioned against the femoral condyle.

64. A system according to claim 63 wherein the second major surface is provided with a femoral glide path to facilitate its performance *in situ*.

65. A system according to claim 64 wherein the glide path is in the form of a generally central oval depression about 1 mm to about 5mm deep at its lowest point and about 30 mm to about 50 mm in length by 10 mm to 30 mm in width.

66. A system according to claim 63 wherein the implant also includes a raised tibial projection adapted to catch the posterior portion of the tibial plateau *in situ*.

67. A system according to claim 63 wherein the implant has dimensions on the order of between about 40 to about 60 mm in the anterior-posterior dimension, between about 30 mm to about 40 mm in the medial-lateral dimension, and a maximum thickness, at the posterior lip, of between about 10 mm and about 20 mm.

68. A system according to claim 63 wherein the preformed component includes ancillary means for securing the component once formed in the joint site.

69. A system according to claim 68 wherein the ancillary means comprise one or more protrusions adapted to be attached to either soft tissue and/or bone at the joint site to improve fixation.

70. A system according to claim 68 wherein the contoured surface of the preformed component further comprises a contour having one or more protrusions, integral with the preformed component, and formed during the *ex vivo* molding process.

71. A system according to claim 70 wherein the protrusions are adapted to be integrated into the preformed component during the *ex vivo* molding process and comprise sutures and/or fibrous biomaterials integrally formed with the component itself.

72. A system according to claim 68 wherein the ancillary means are selected from the group consisting of adhesives, sutures, pins, staples, screws, and combinations thereof.

73. A system according to claim 70 wherein the implant is preformed in a mold having an anterior cup edge that is substantially perpendicular to the plane of the cup itself, and a posterior mesial edge that is tapered and raised to accommodate the corresponding shape of the tibial spine.

74. A system according to claim 73 wherein the mold is adapted to permits control of sizing, conformance to the joint site, implant thickness and angular correction.

75. A system according to claim 74 where the implant assumes a generally kidney-shaped configuration, adapted to correspond with the tibial surface, and provides a posterior mesial edge portion having an indentation to accommodate the typical shape of the corresponding tibial spine.

76. A system according to claim 15 wherein the polyurethane comprises an isocyanate selected from the group consisting of aromatic, aliphatic and arylakyl diisocyanates, and combinations thereof.

77. A system according to claim 76 wherein the isocyanate is selected from the group consisting of toluene diisocyanates, naphthalene diisocyanates, phenylene diisocyanates, xylylene diisocyanates, diphenylmethane diisocyanates, cyclohexane diisocyanates, cyclohexylbis methylene diisocyanates, isophorone diisocyanates and hexamethylene diisocyanates.

78. A system according to claim 63 further comprising a patella-femoral joint form suitable adapted to be formed to, and held against, the femoral bone surface, in order to permit the delivery of curable biopolymer between the form and the bone.

79. A system according to claim 1 wherein the implant is provided in the form of a preformed knee implant prepared using an *ex vivo* mold and having a first major surface adapted to be positioned upon the tibial surface, and a second major surface adapted to be positioned against the femoral condyle, the implant also includes a raised tibial projection adapted to catch the posterior portion of the tibial plateau *in situ*, the implant has dimensions on the order of between about 40 to about 60 mm in the anterior-posterior dimension, between about 30 mm to about 40 mm in the medial-lateral dimension, and a maximum thickness, at the posterior lip, of

between about 10 mm and about 20 mm, the preformed component includes ancillary means for securing the component once formed in the joint site, and the preformed component is fabricated from a polyurethane that comprises an isocyanate comprising a phenylene diisocyanate.

10098504-031502

ABSTRACT

A method and system for the creation or modification of the wear surface of orthopedic joints, involving the preparation and use of one or more partially or fully preformed and procured components, adapted for insertion and placement into the body and at the joint site. In a preferred embodiment, component(s) can be partially cured and generally formed *ex vivo* and further and further formed *in vivo* at the joint site to enhance conformance and improve long term performance. In another embodiment, a preformed balloon or composite material can be inserted into the joint site and filled with a flowable biomaterial in situ to conform to the joint site. In yet another embodiment, the preformed component(s) can be fully cured and formed *ex vivo* and optionally further fitted and secured at the joint site. Preformed components can be sufficiently pliant to permit insertion through a minimally invasive portal, yet resilient enough to substantially assume, or tend towards, the desired form *in vivo* with additional forming there as needed.

2025 FEB 10 09:56 AM

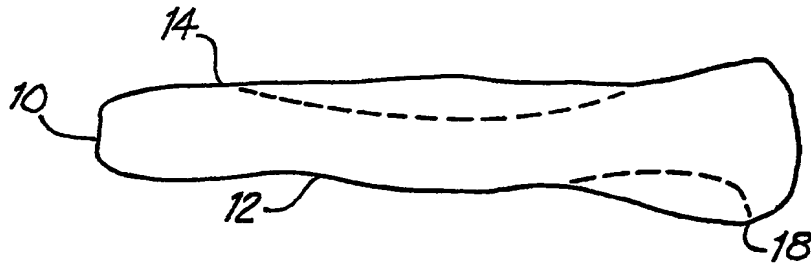


FIG. 1a

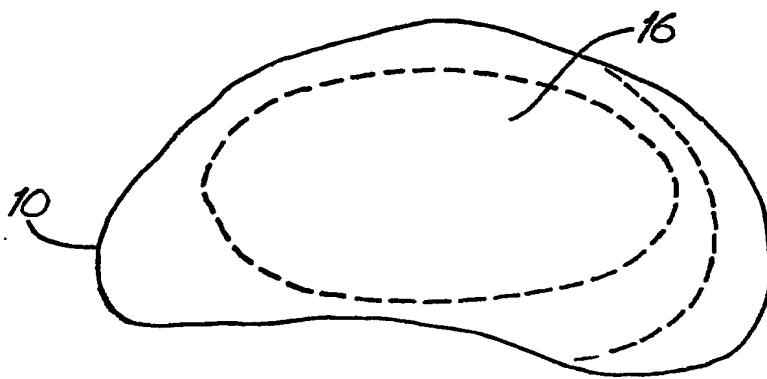


FIG. 1b

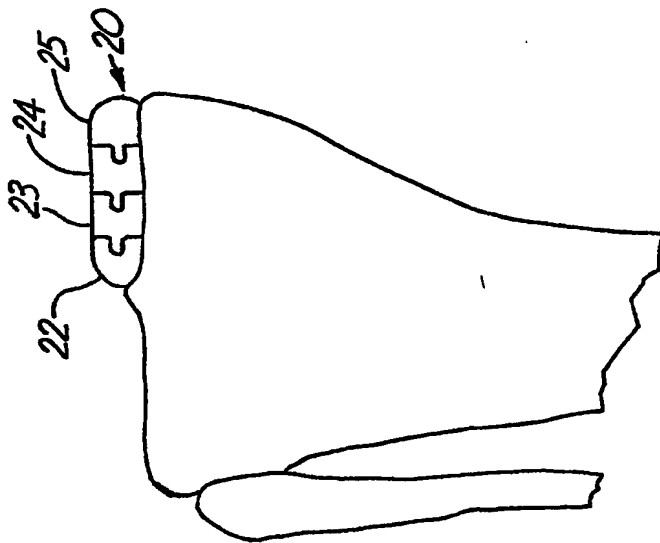


FIG. 2a

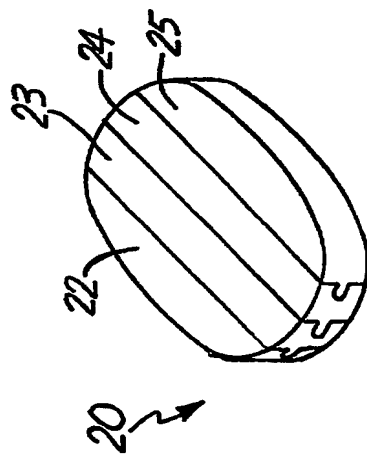
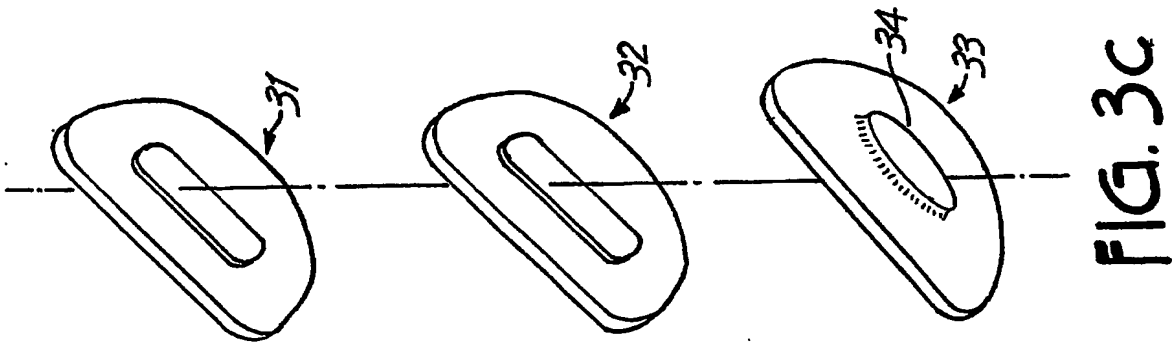
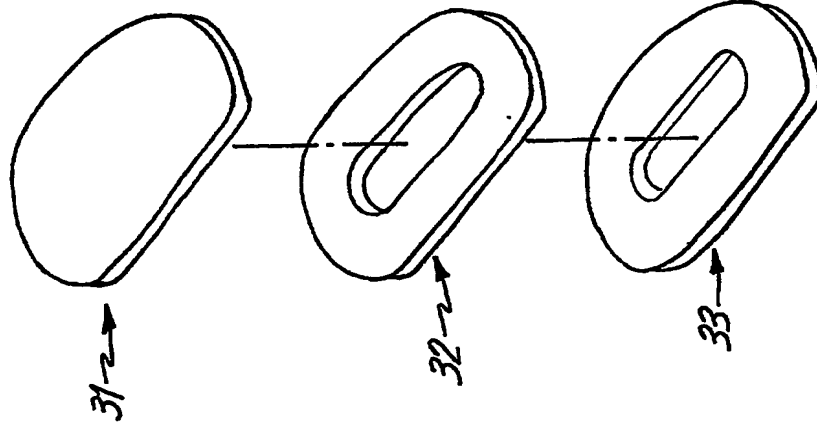
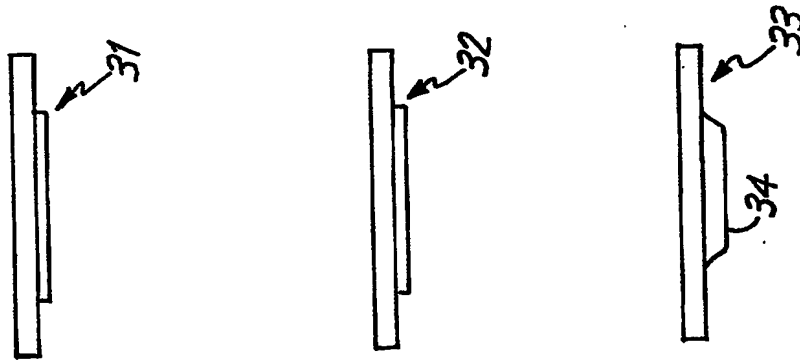


FIG. 2b



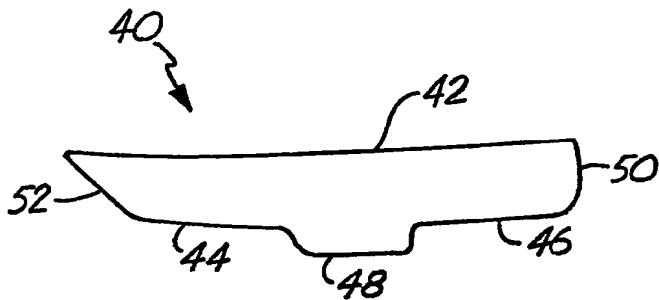


FIG. 4a

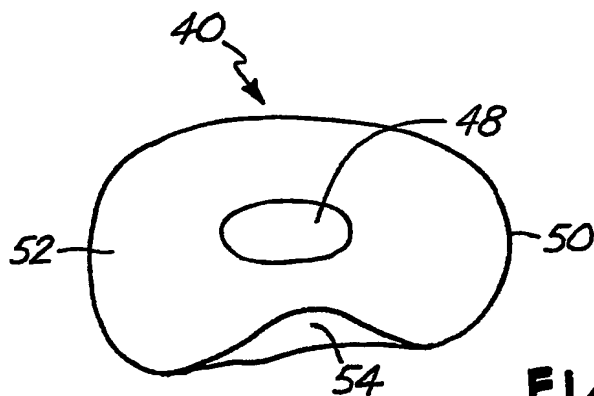


FIG. 4b

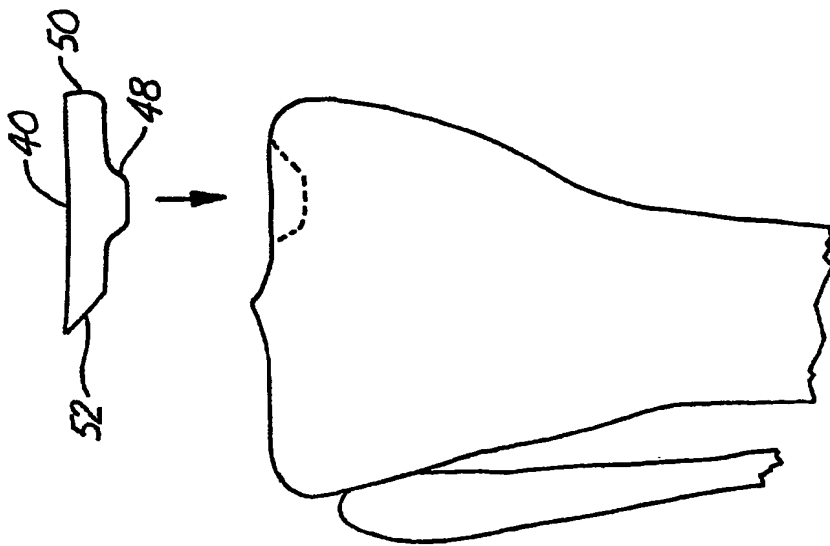


FIG. 5a

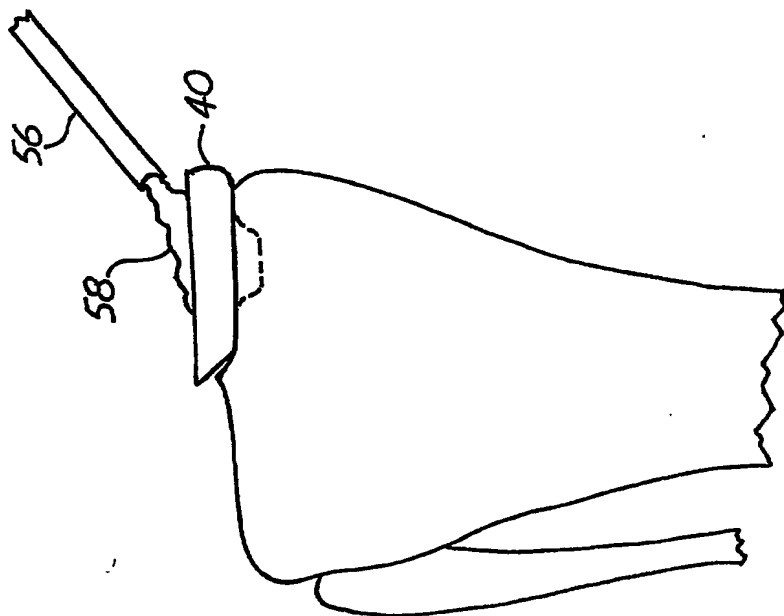


FIG. 5b



FIG. 6a

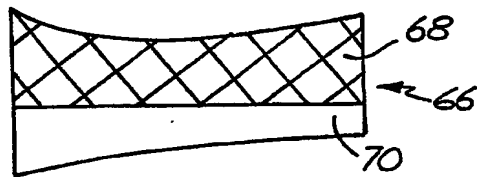


FIG. 6b

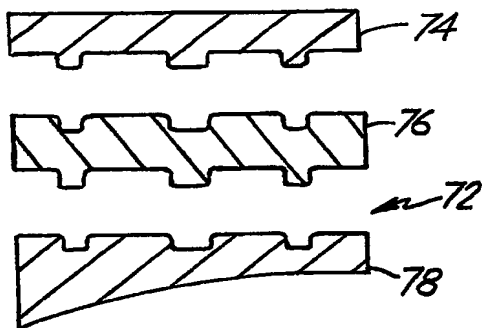


FIG. 6c

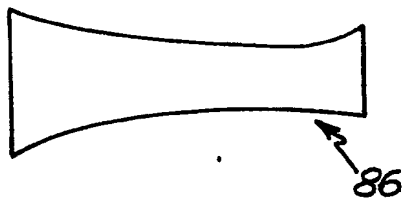


FIG. 6d

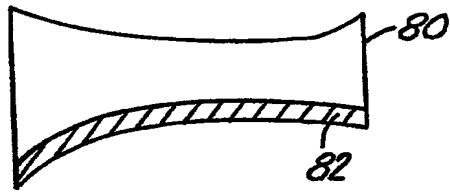


FIG. 7a

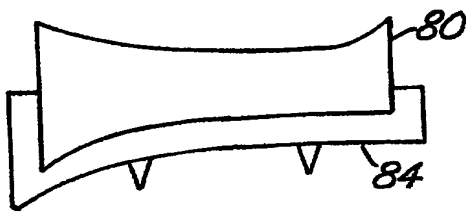


FIG. 7b

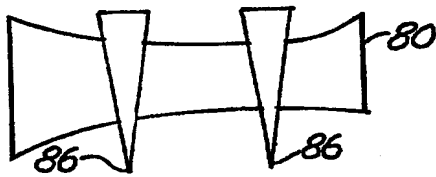


FIG. 7c

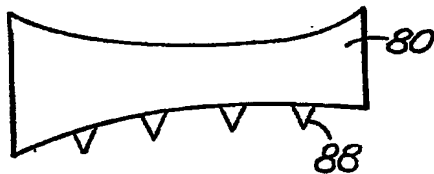


FIG. 7d

8/11

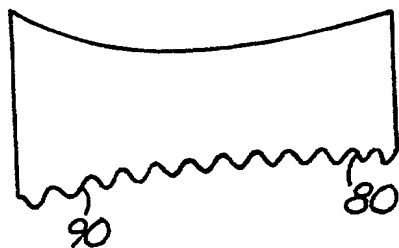


FIG. 8a

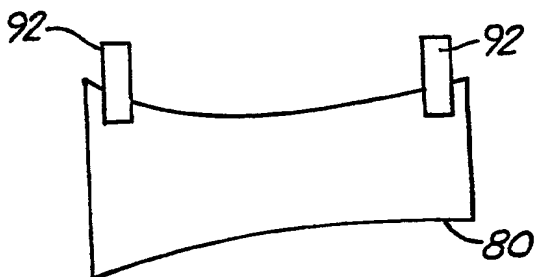


FIG. 8b

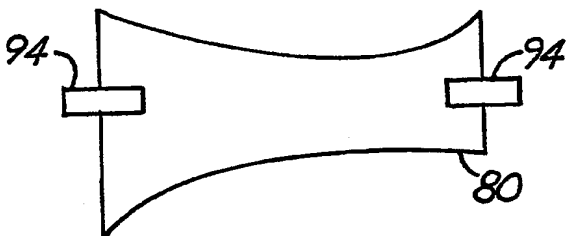


FIG. 8c

202507098601.031502

9/11

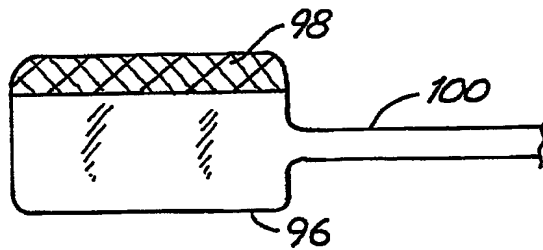


FIG. 9a

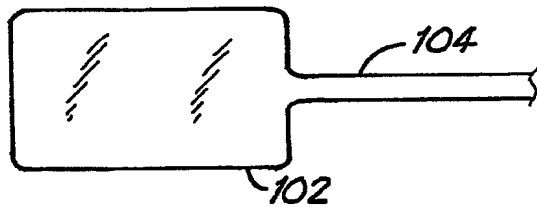


FIG. 9b

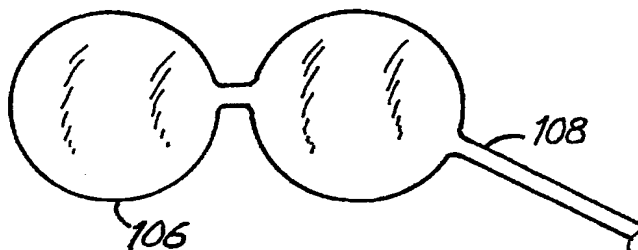


FIG. 9c

202501-031502

20570709800T 10098601.031502





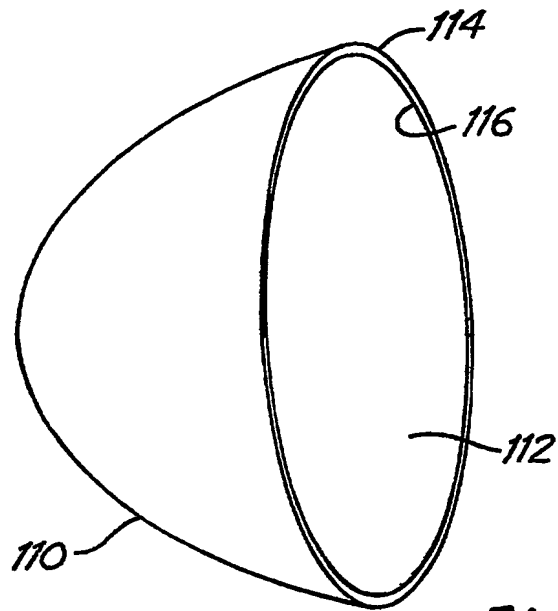


FIG. 10

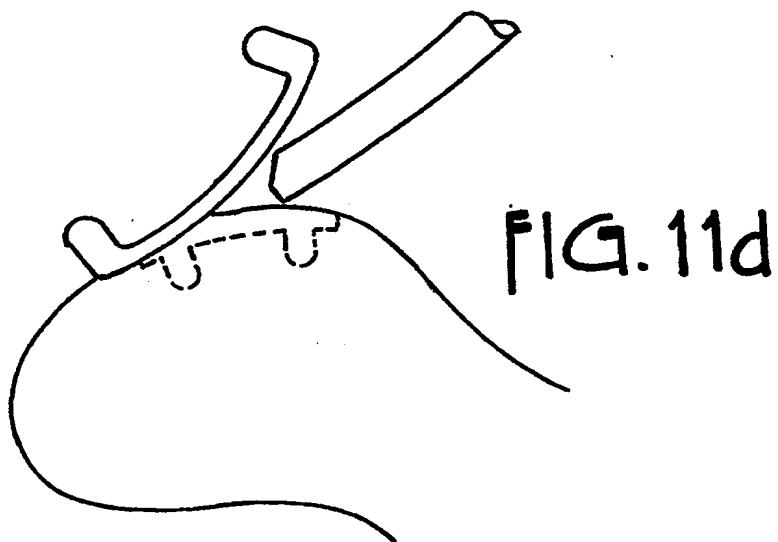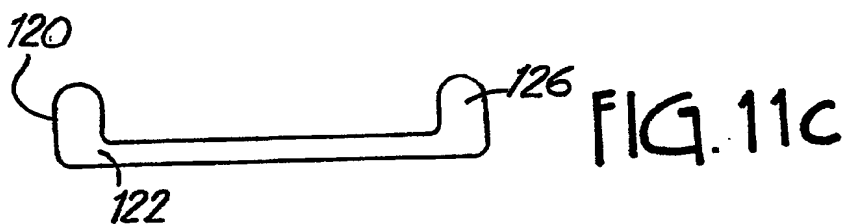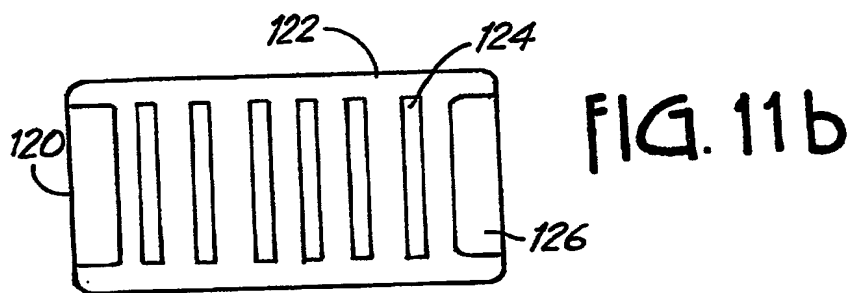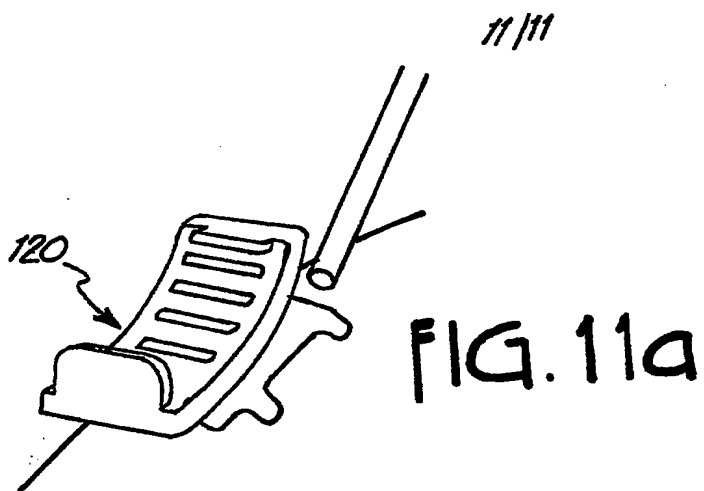

10099601.031502

**This Page is Inserted by IFW Indexing and Scanning
Operations and is not part of the Official Record**

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☒ **BLACK BORDERS**
- ☐ **IMAGE CUT OFF AT TOP, BOTTOM OR SIDES**
- ☐ **FADED TEXT OR DRAWING**
- ☐ **BLURRED OR ILLEGIBLE TEXT OR DRAWING**
- ☐ **SKEWED/SLANTED IMAGES**
- ☐ **COLOR OR BLACK AND WHITE PHOTOGRAPHS**
- ☐ **GRAY SCALE DOCUMENTS**
- ☐ **LINES OR MARKS ON ORIGINAL DOCUMENT**
- ☐ **REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY**
- ☐ **OTHER:** _____

IMAGES ARE BEST AVAILABLE COPY.

As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.